

This Page Is Inserted by IFW Operations
and is not a part of the Official Record

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.


Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

**As rescanning documents *will not* correct images,
please do not report the images to the
Image Problem Mailbox.**

FIG. 1

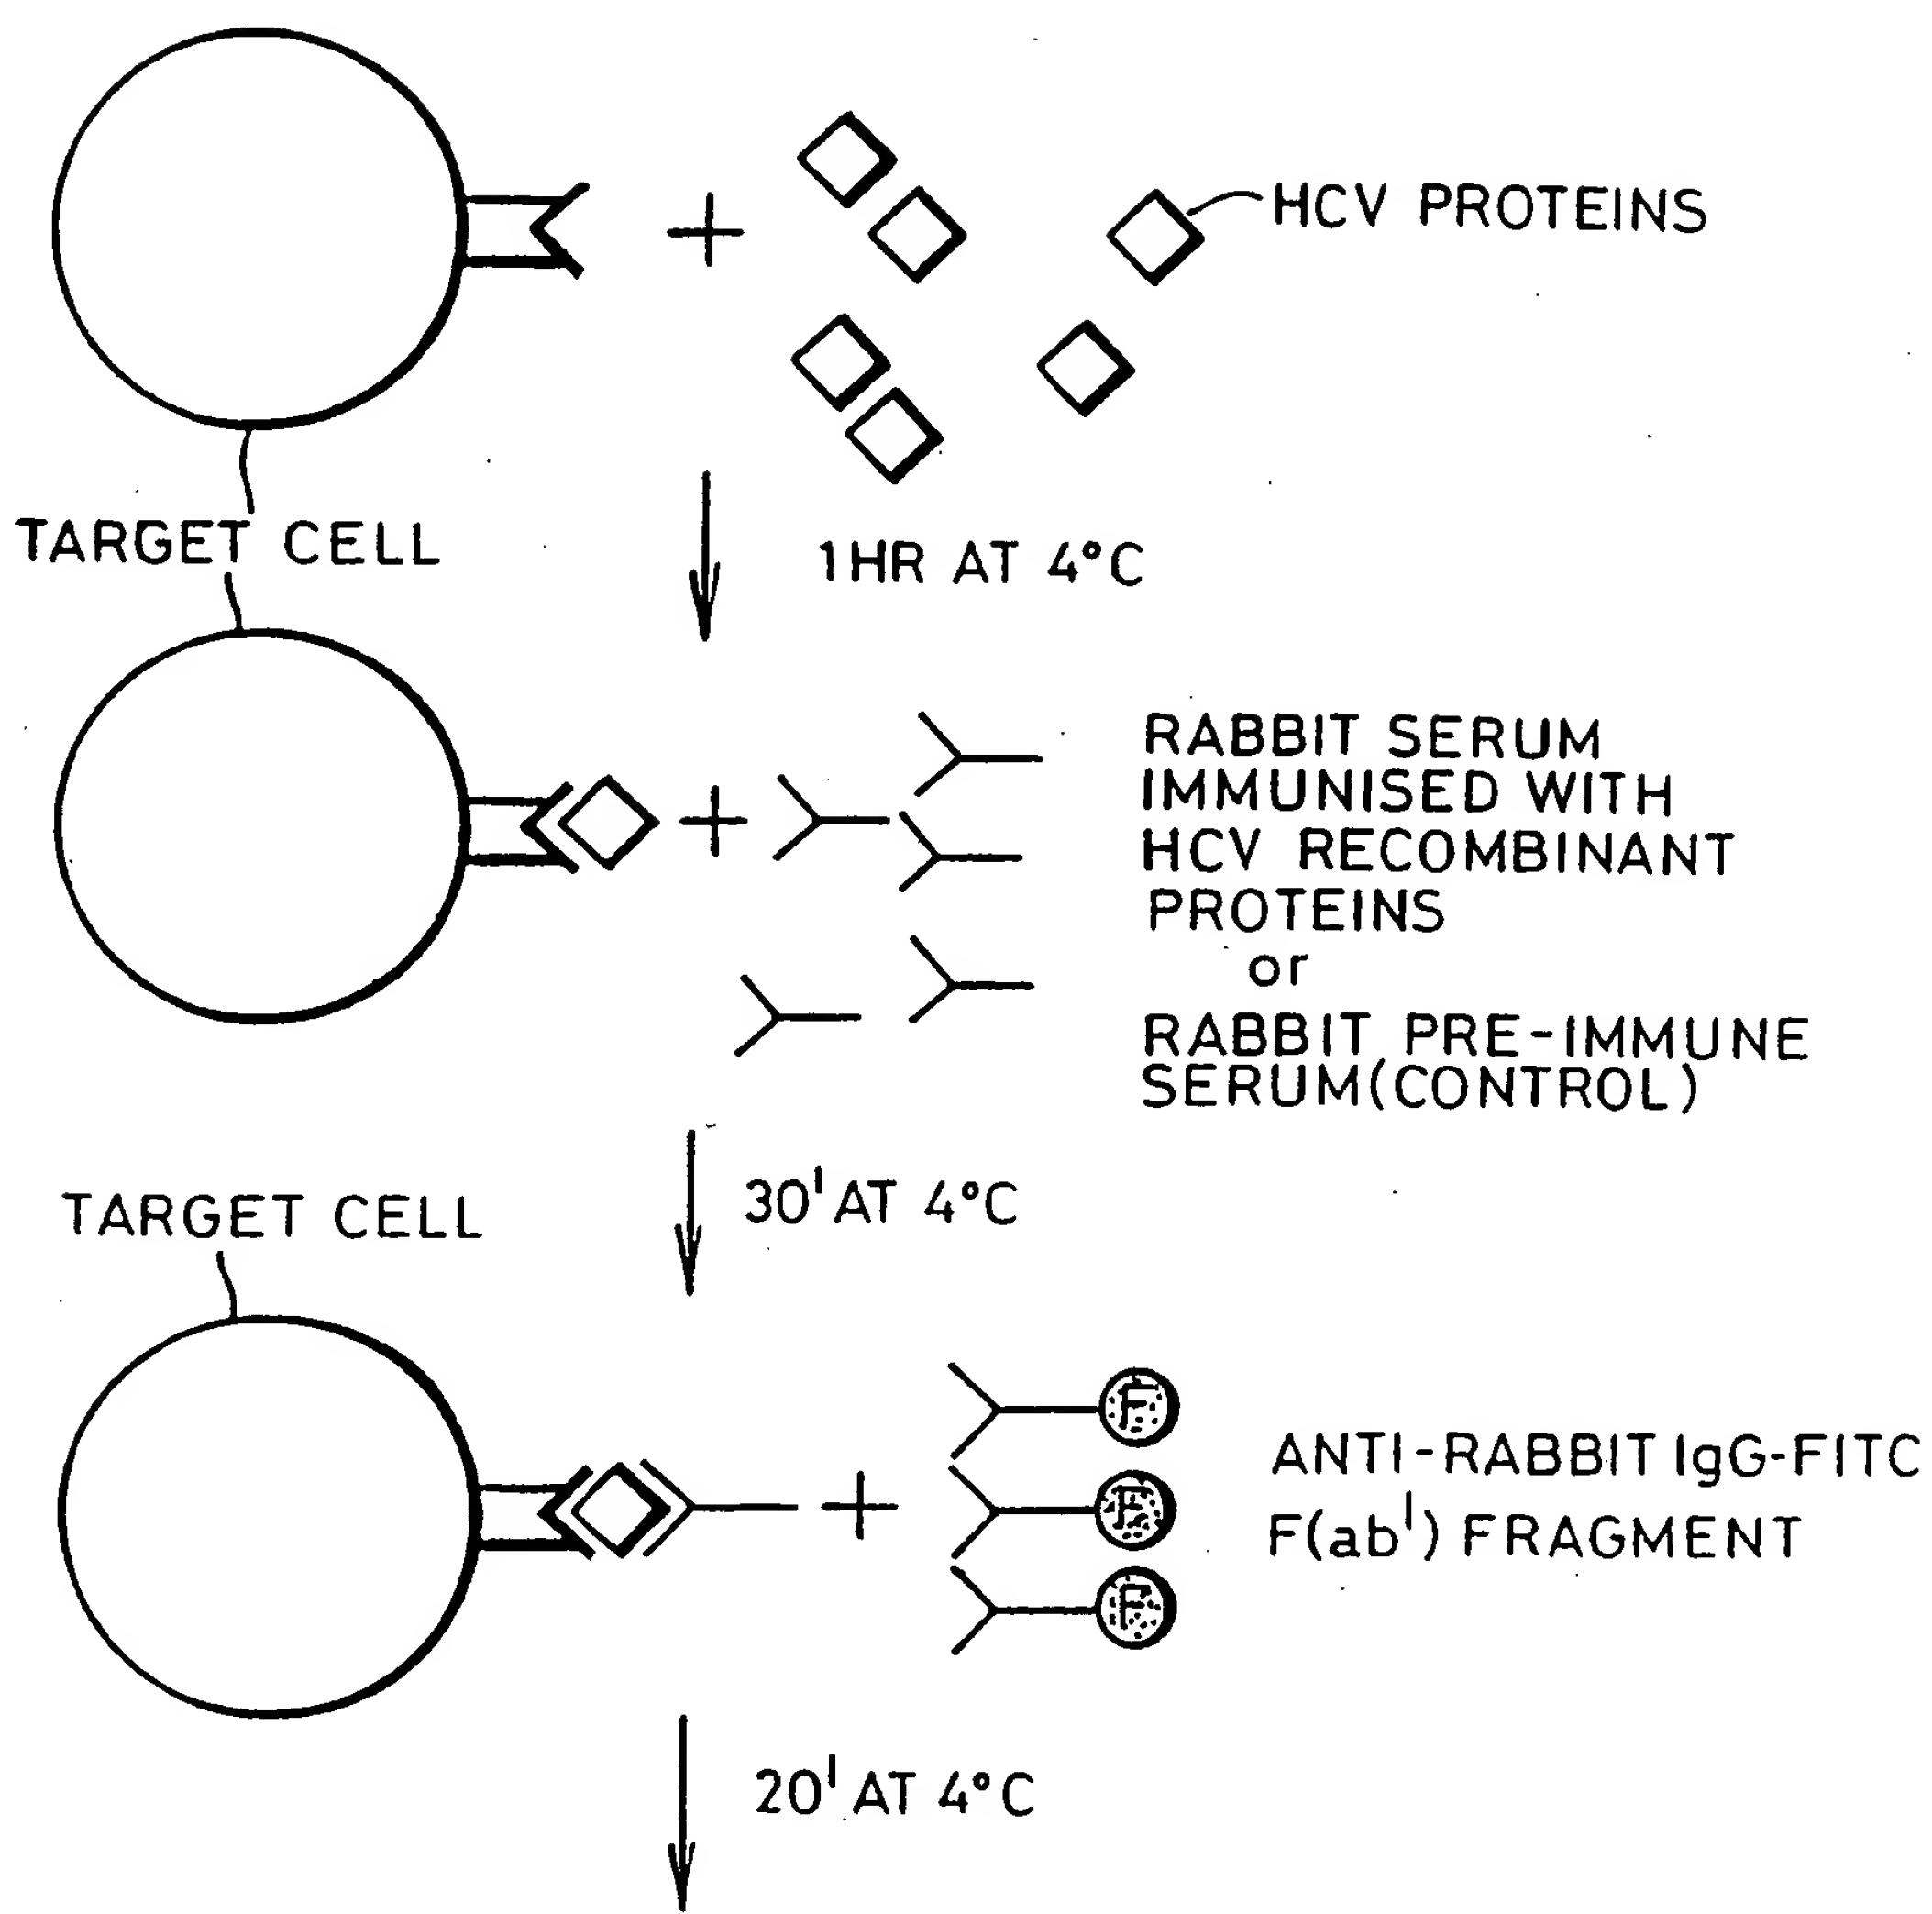

FACScan ANALYSIS

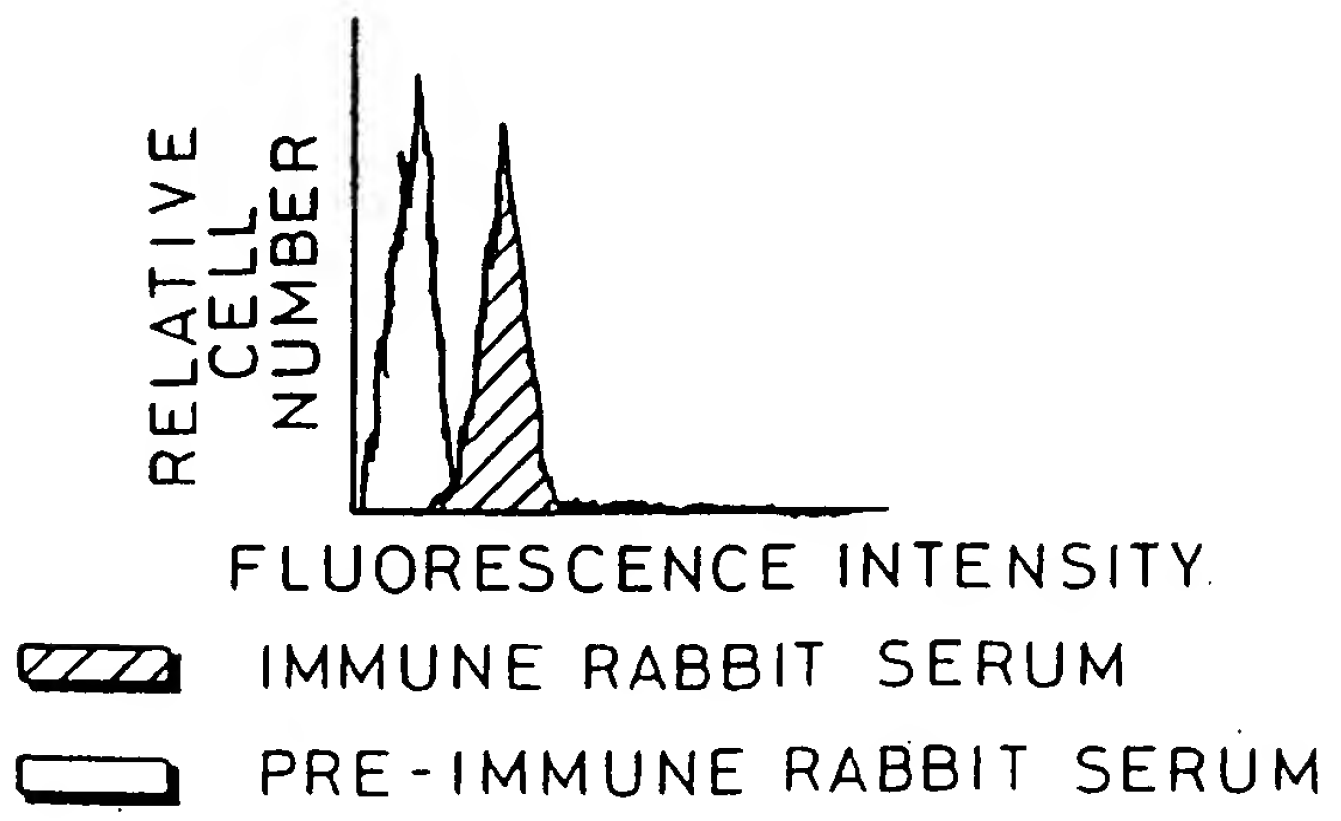




FIG. 2(A)

MOLT 4

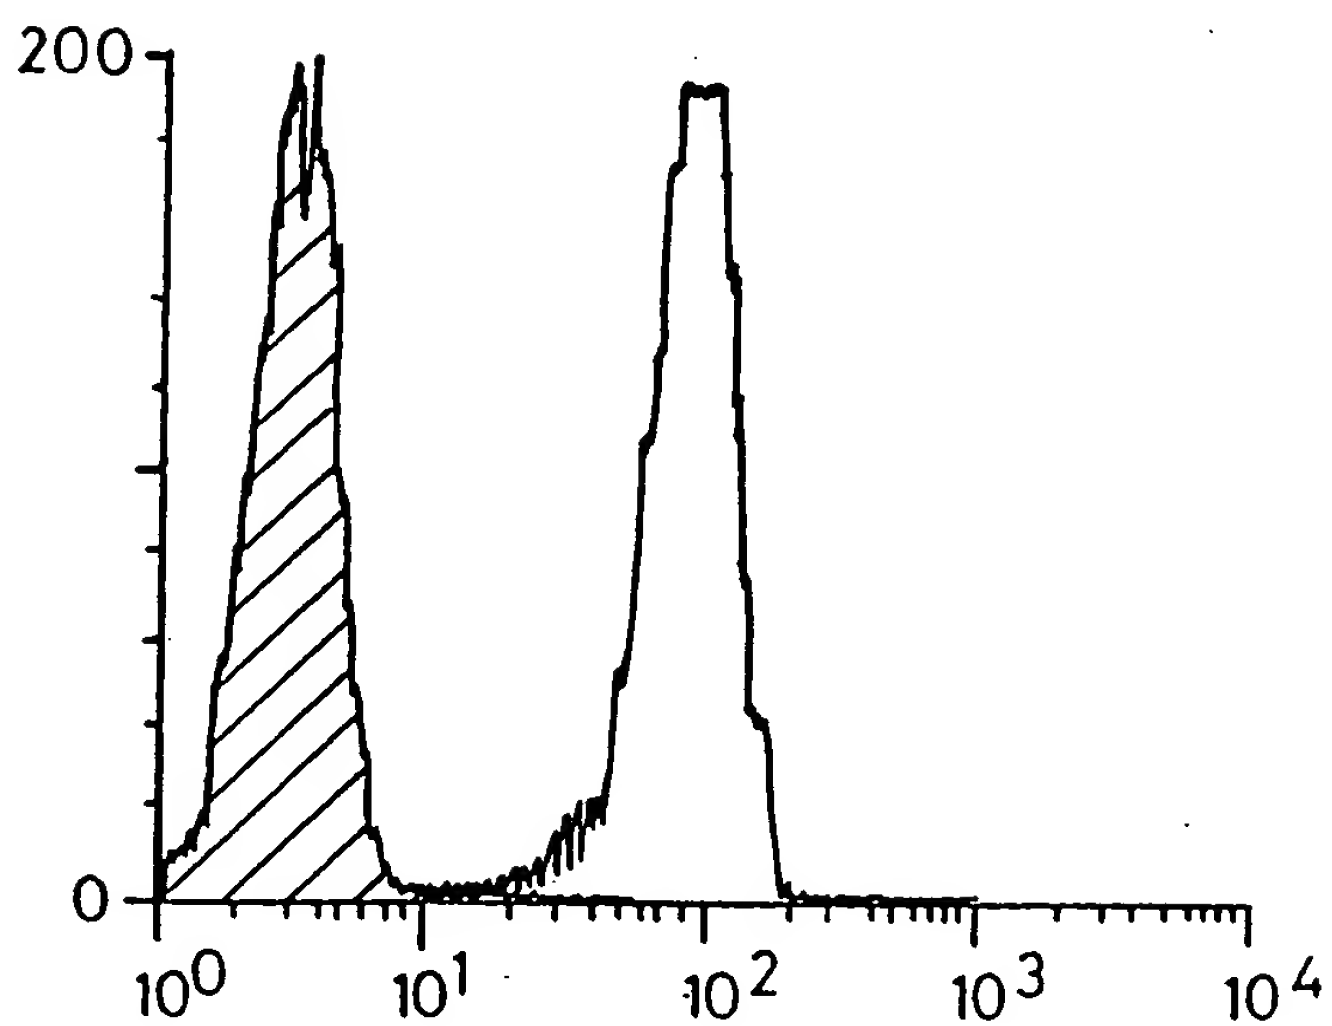
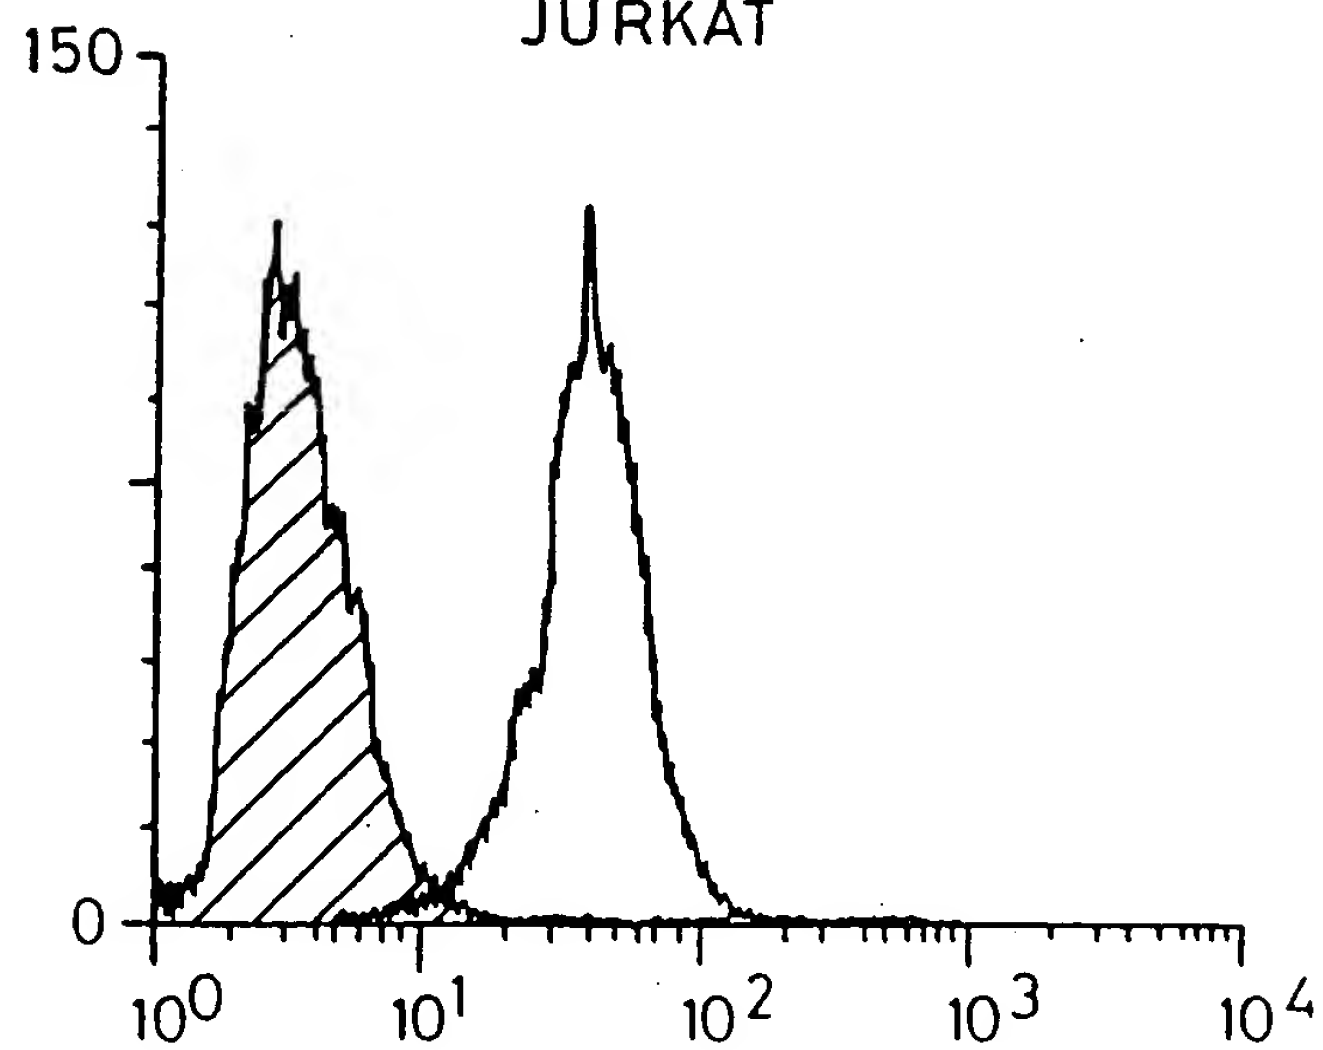


FIG. 2(B)

JURKAT



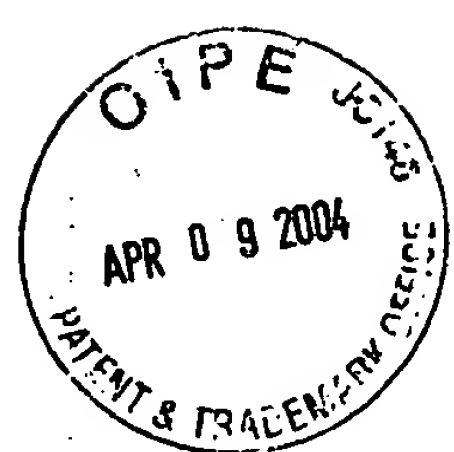


FIG. 2(C)

K562

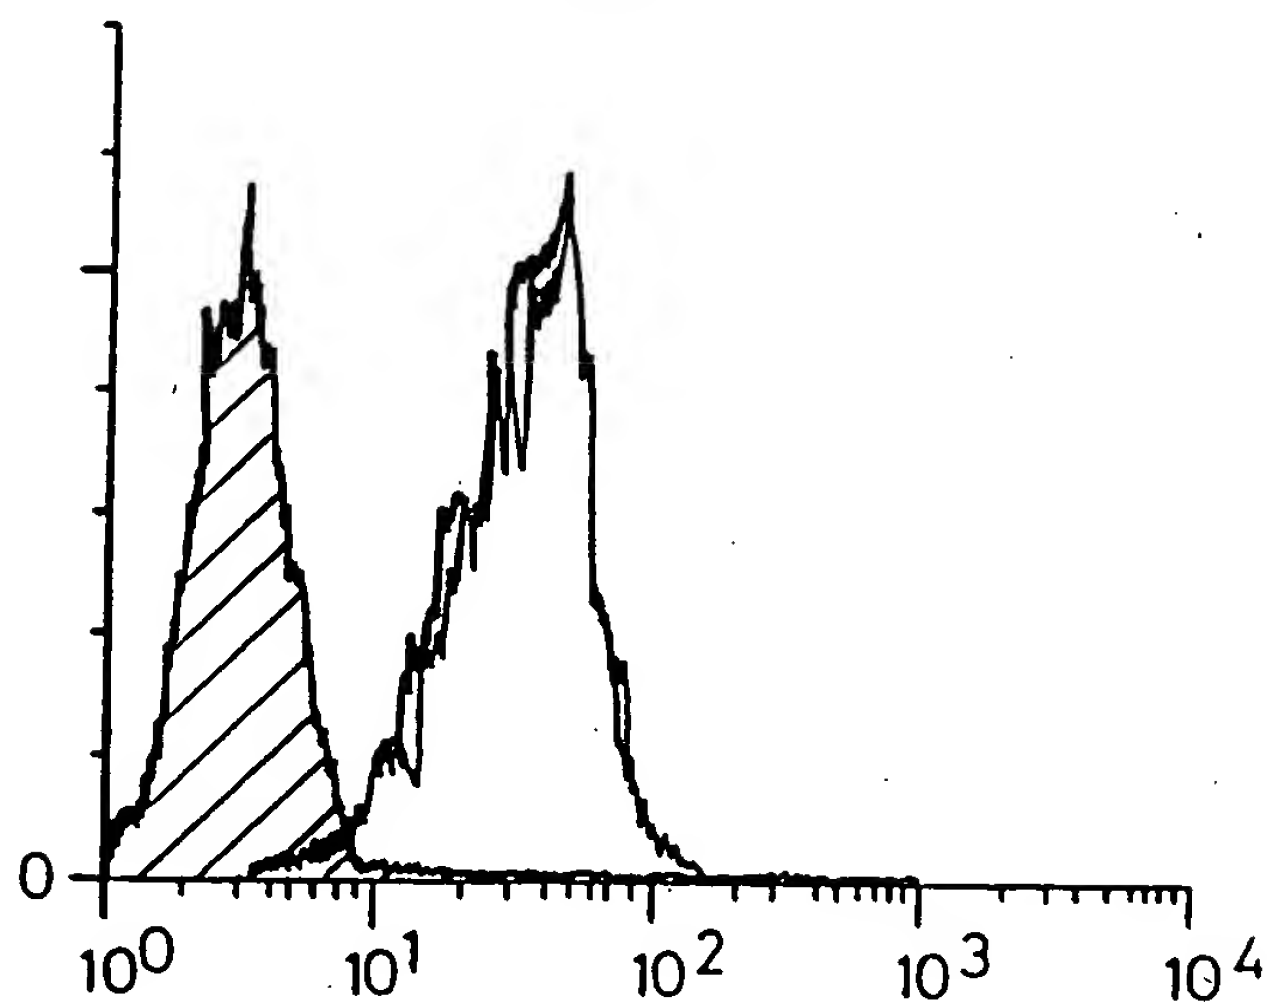
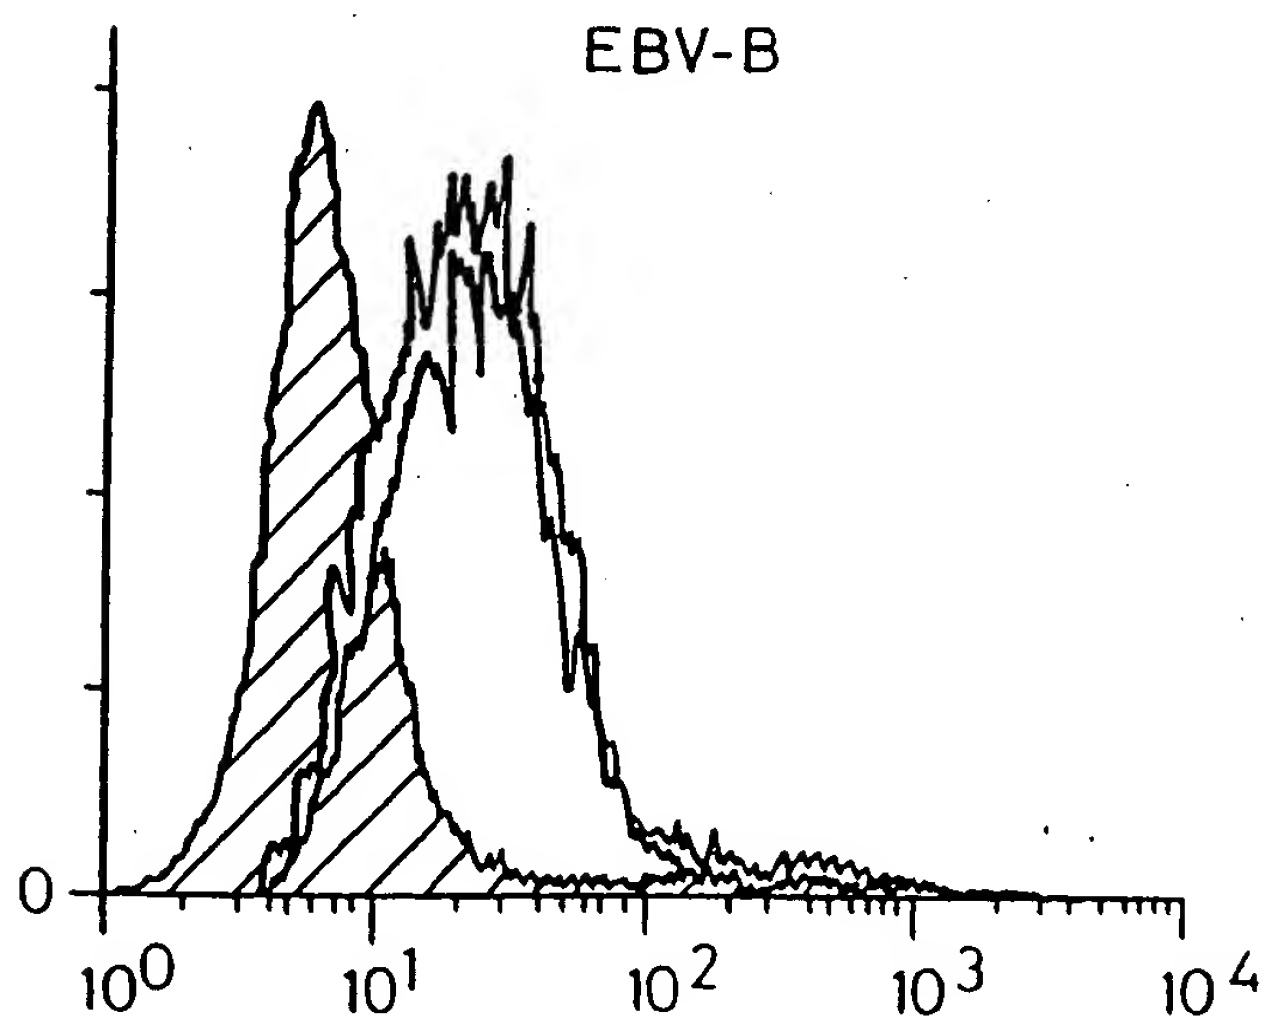


FIG. 2(D)

EBV-B



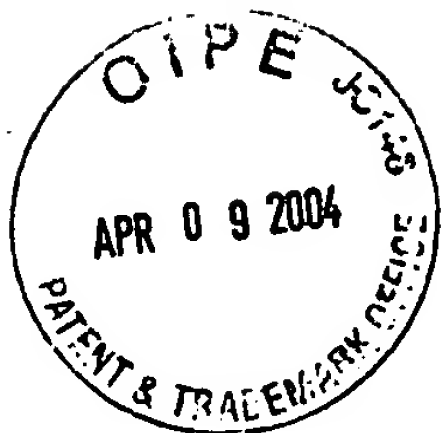


FIG.2(E)

DAUDI

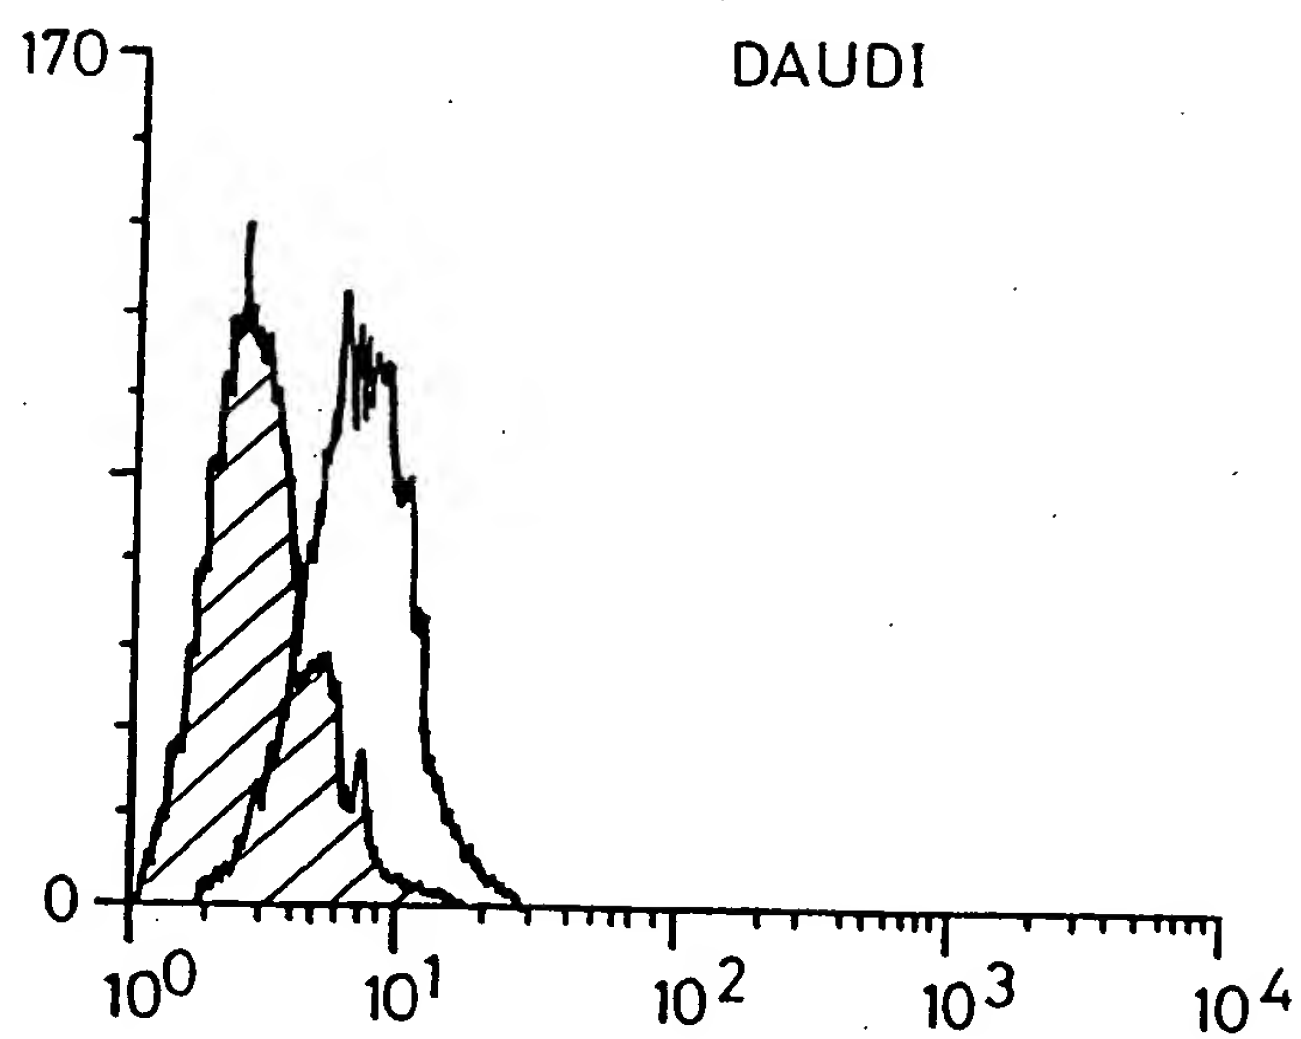


FIG.2(F)

HELA

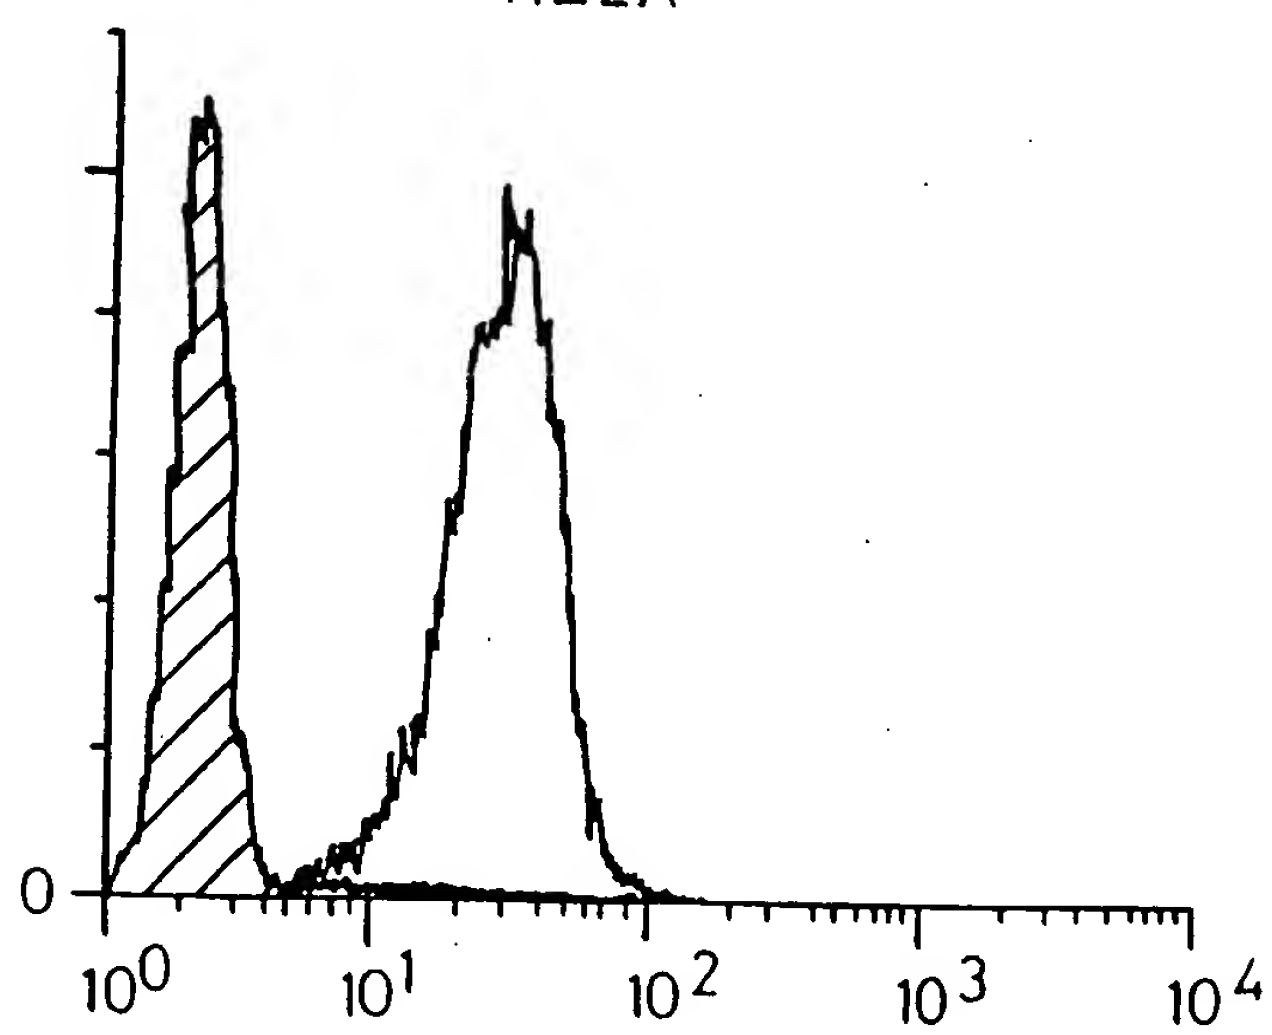




FIG. 2(G)
ADENOCARCINOMA

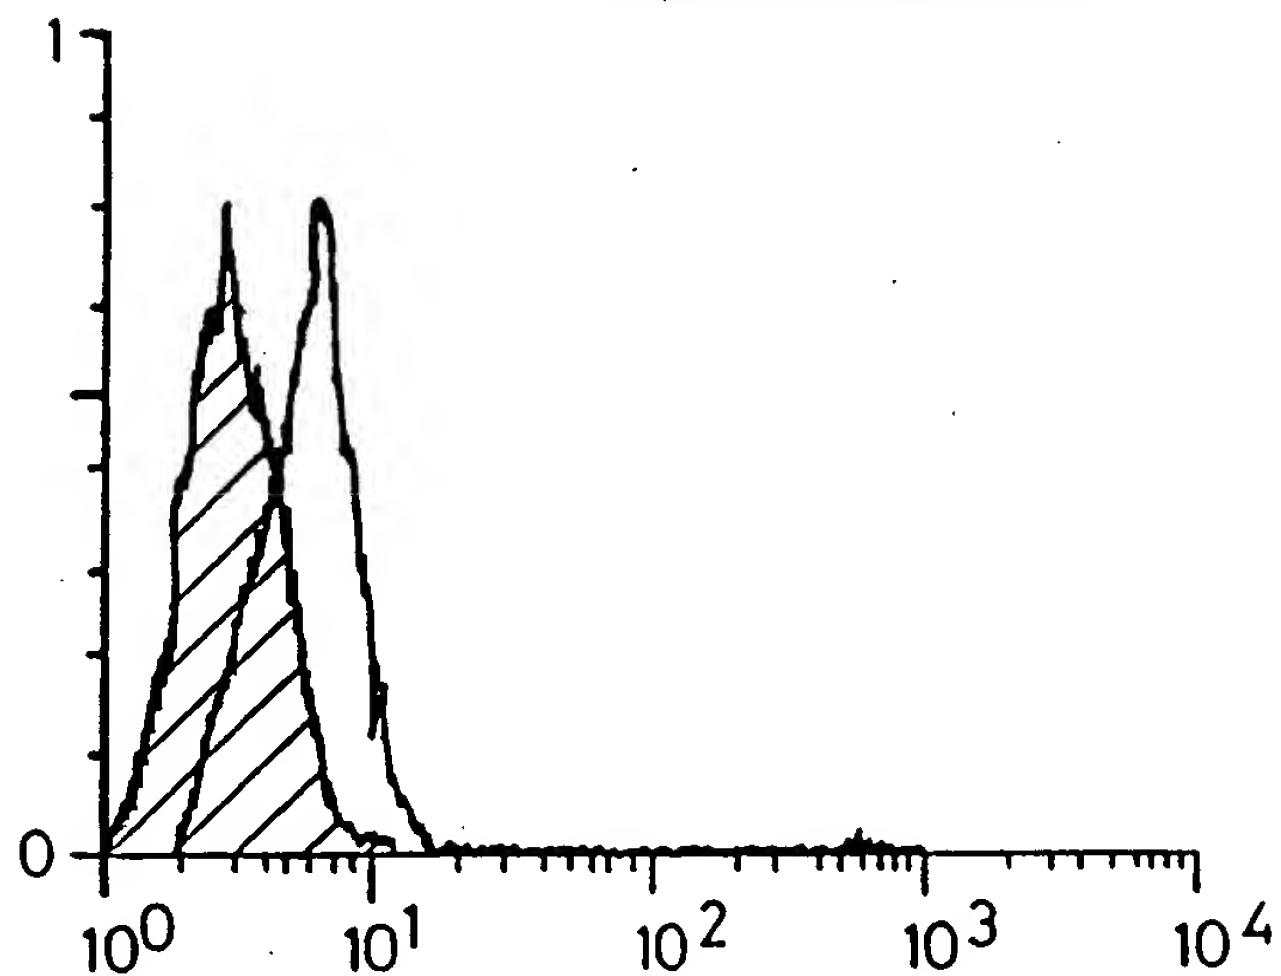
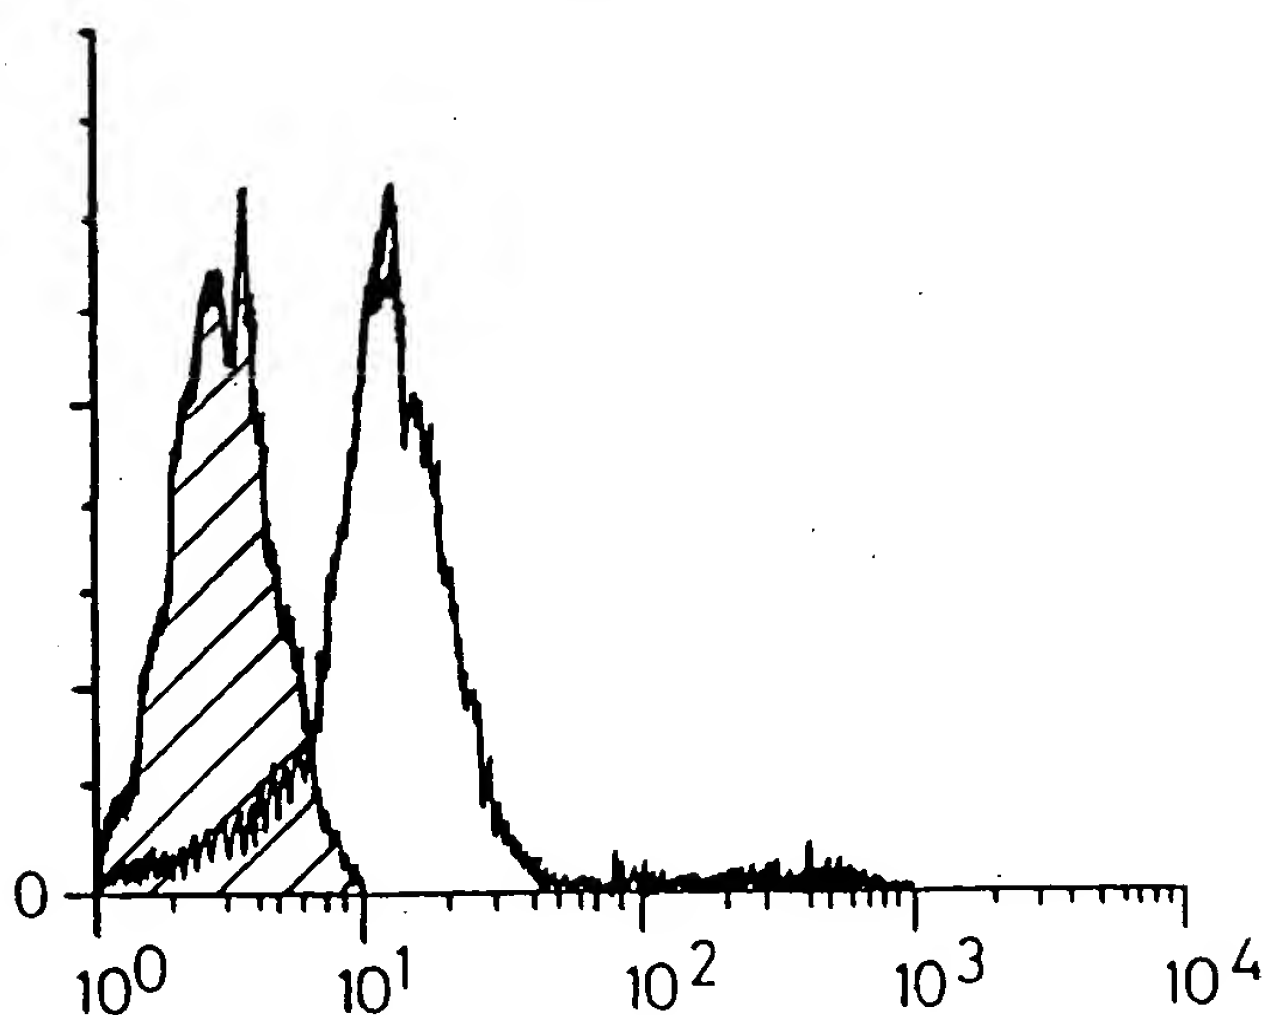


FIG. 2(H)
HUH 7



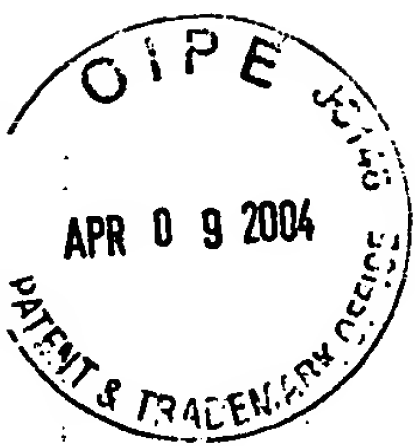


FIG. 3(A)

PURIFIED RA

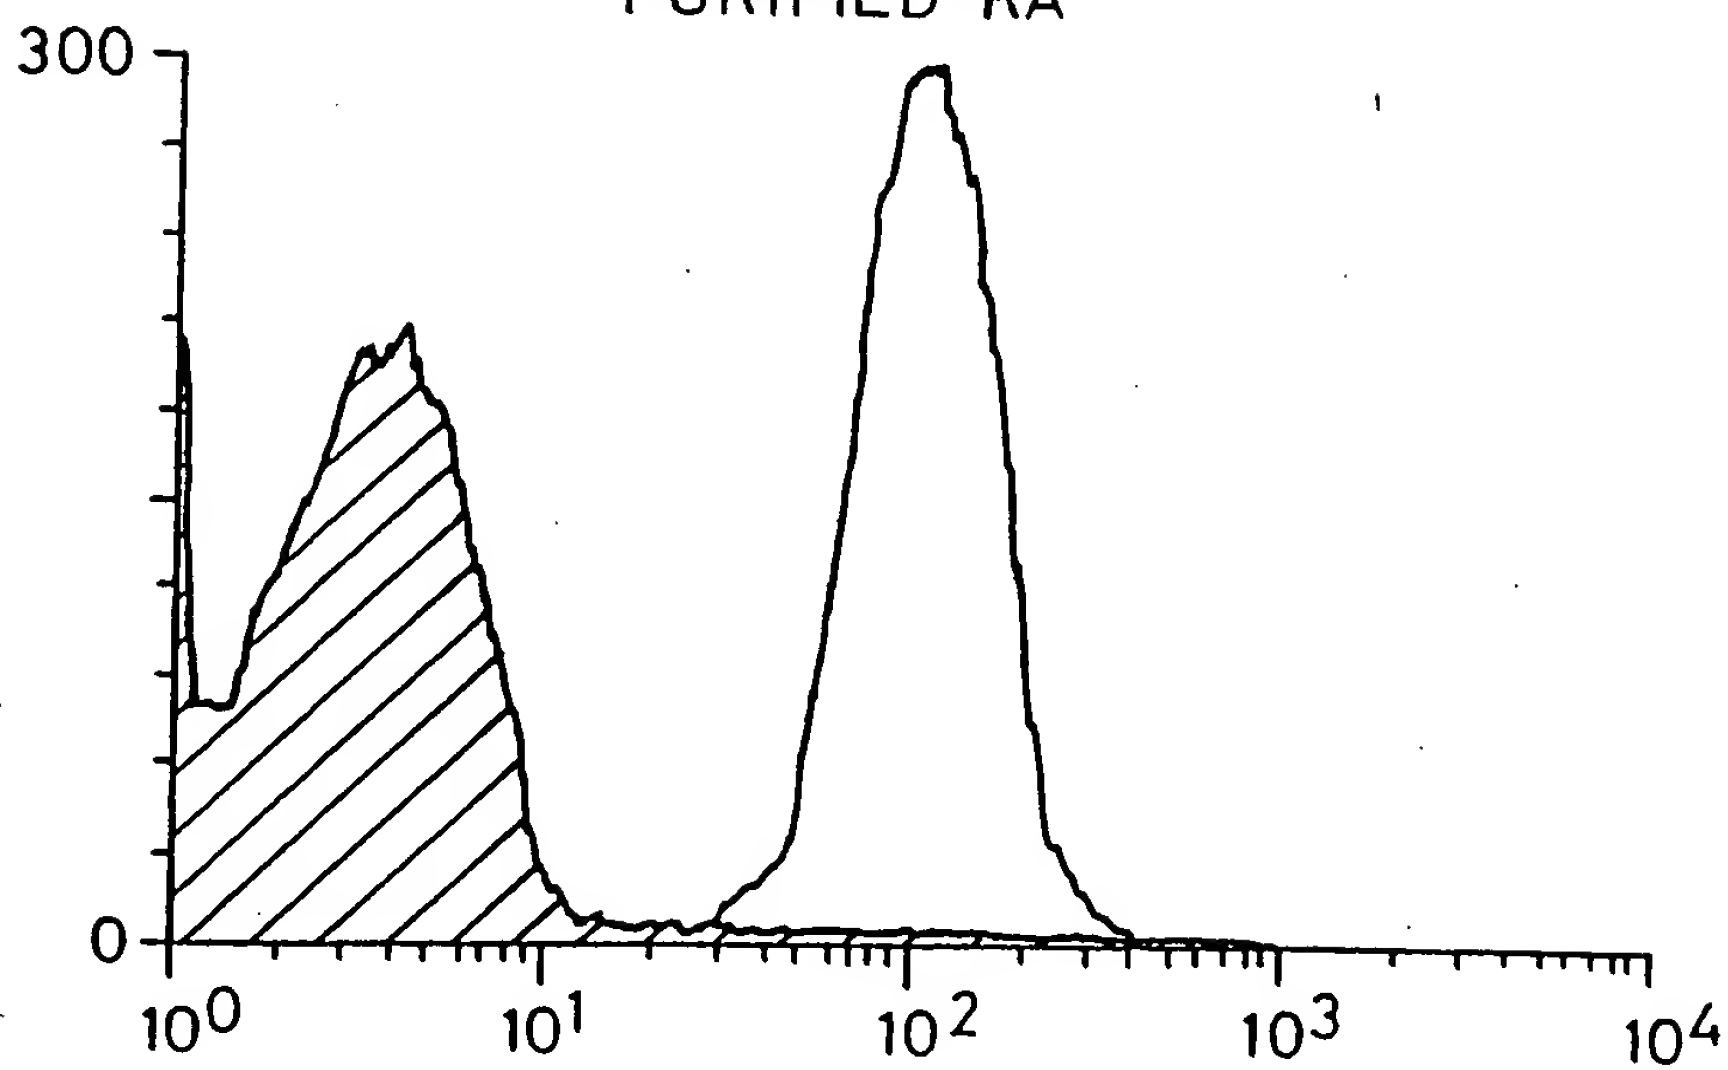


FIG. 3(B)

PURIFIED RO

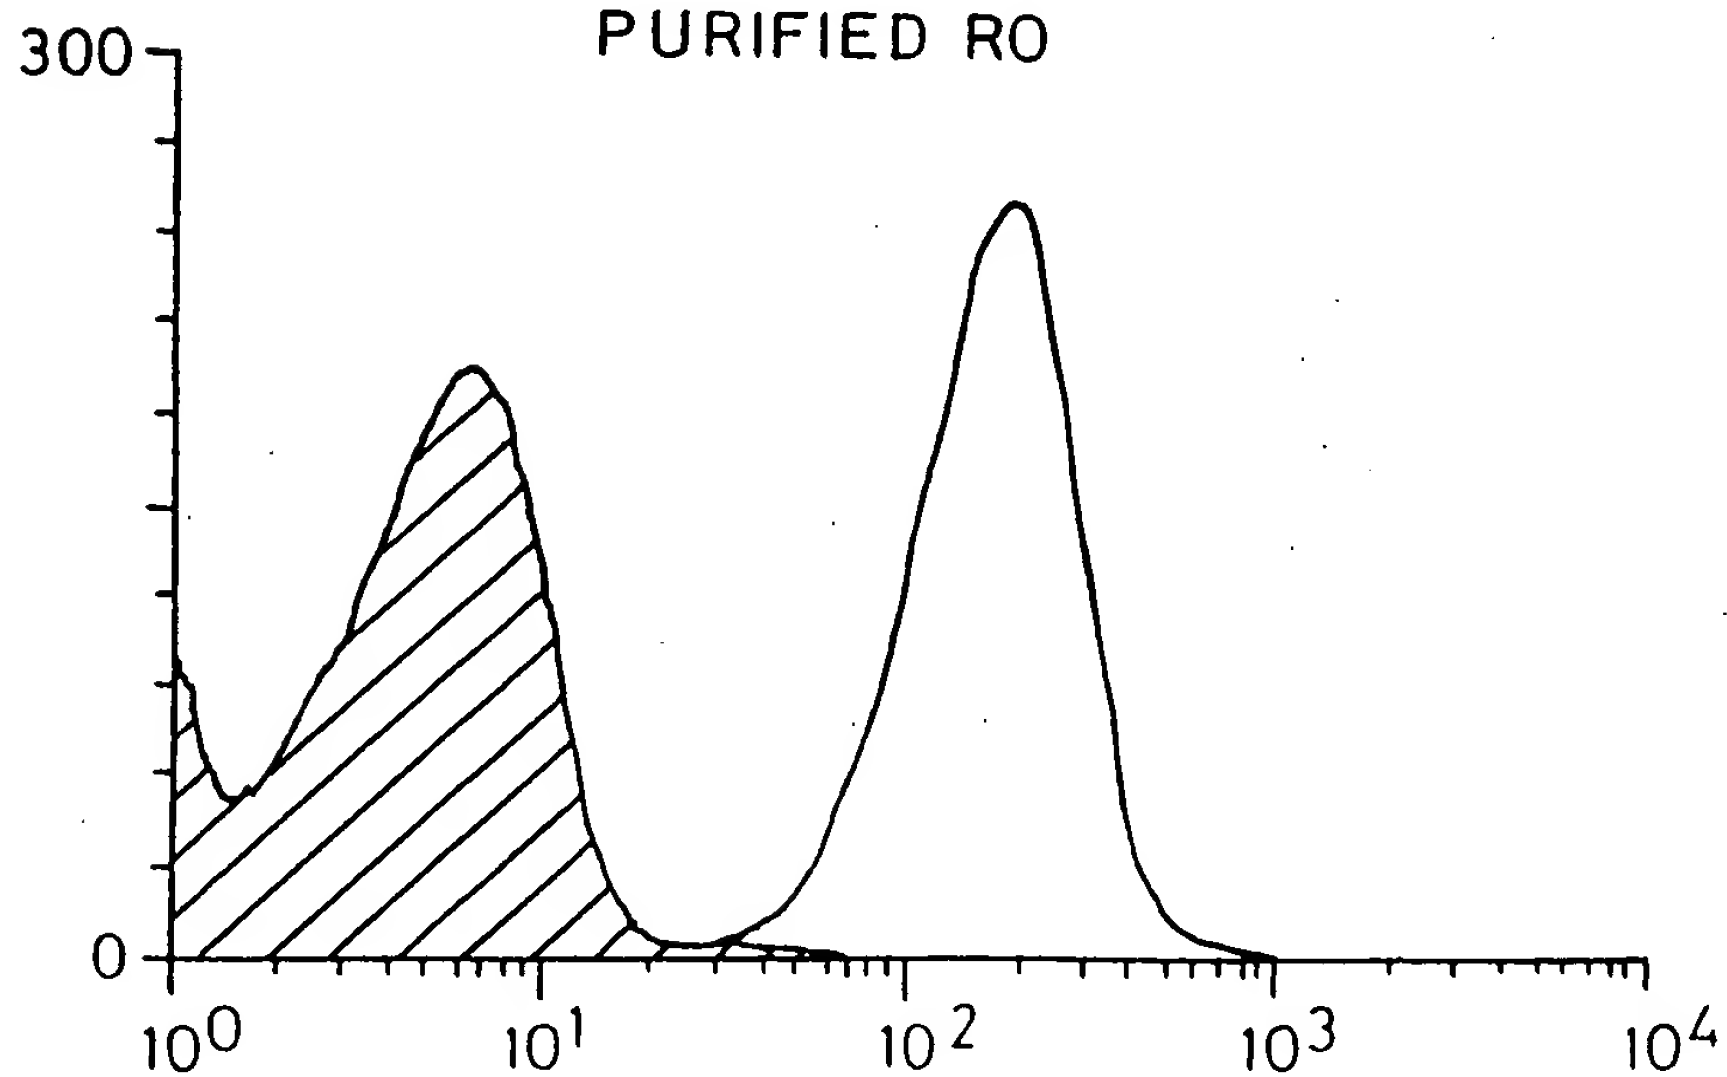




FIG. 3(C)

CORD BLOOD PURIF. RA

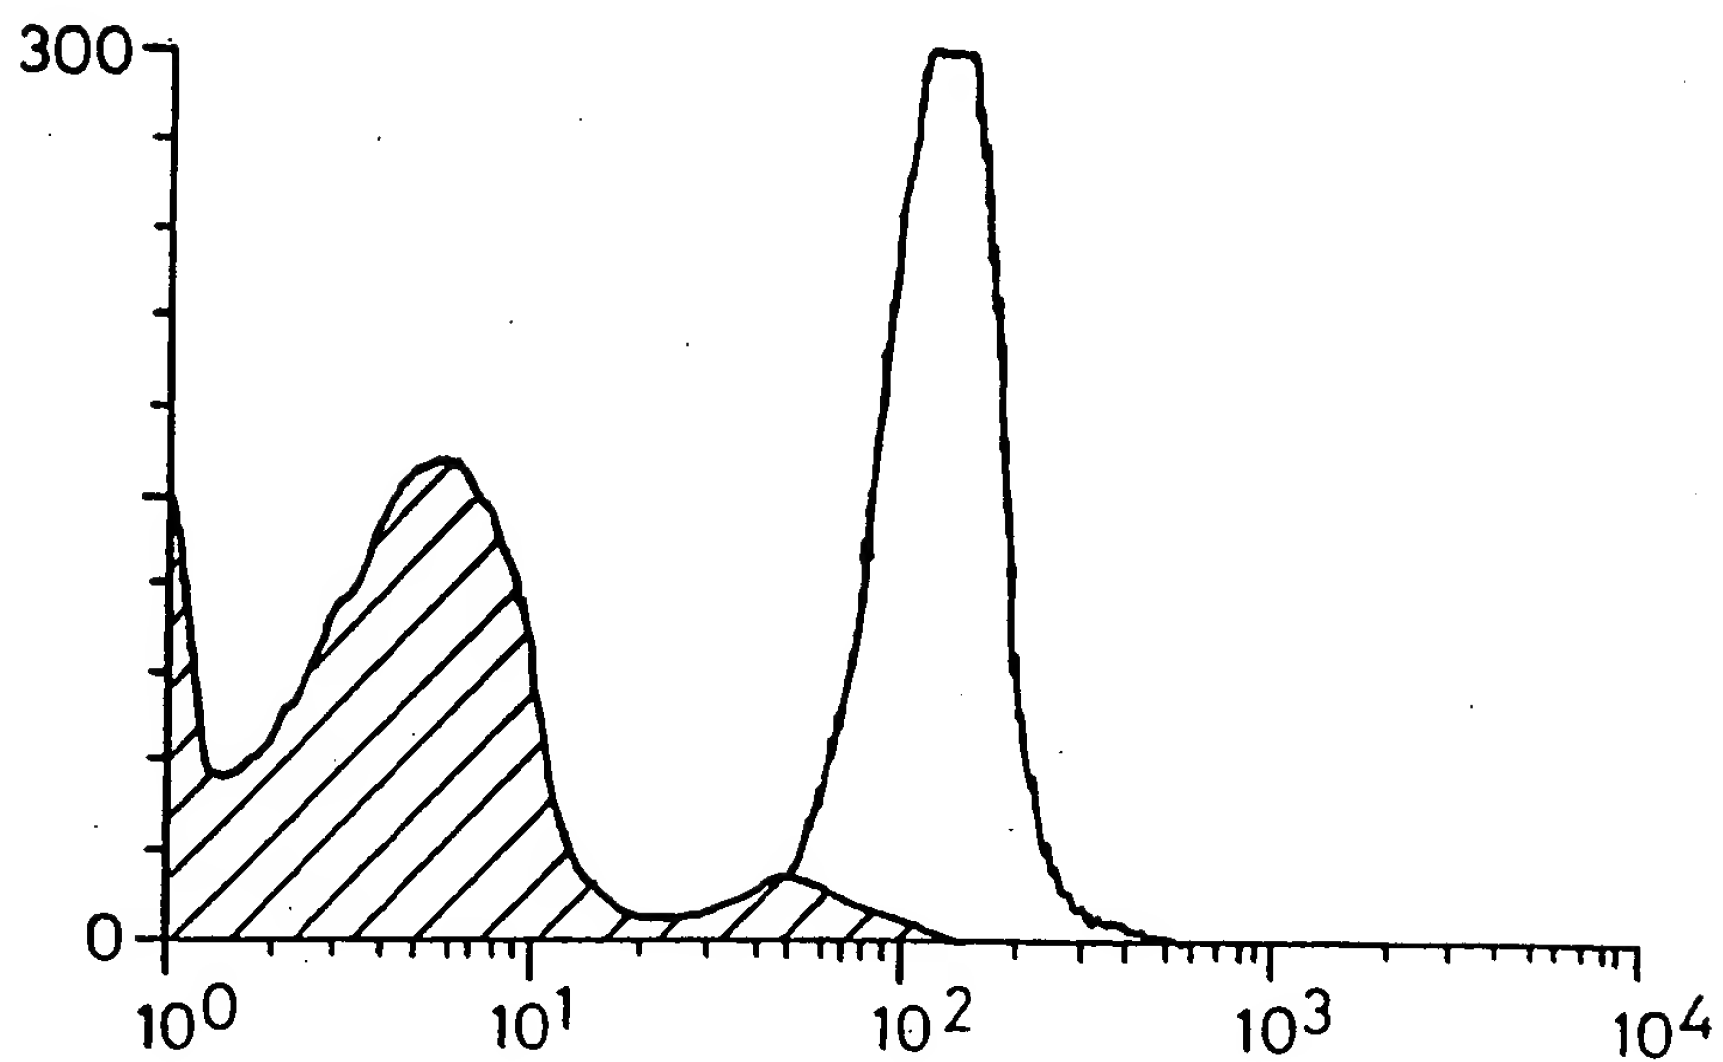
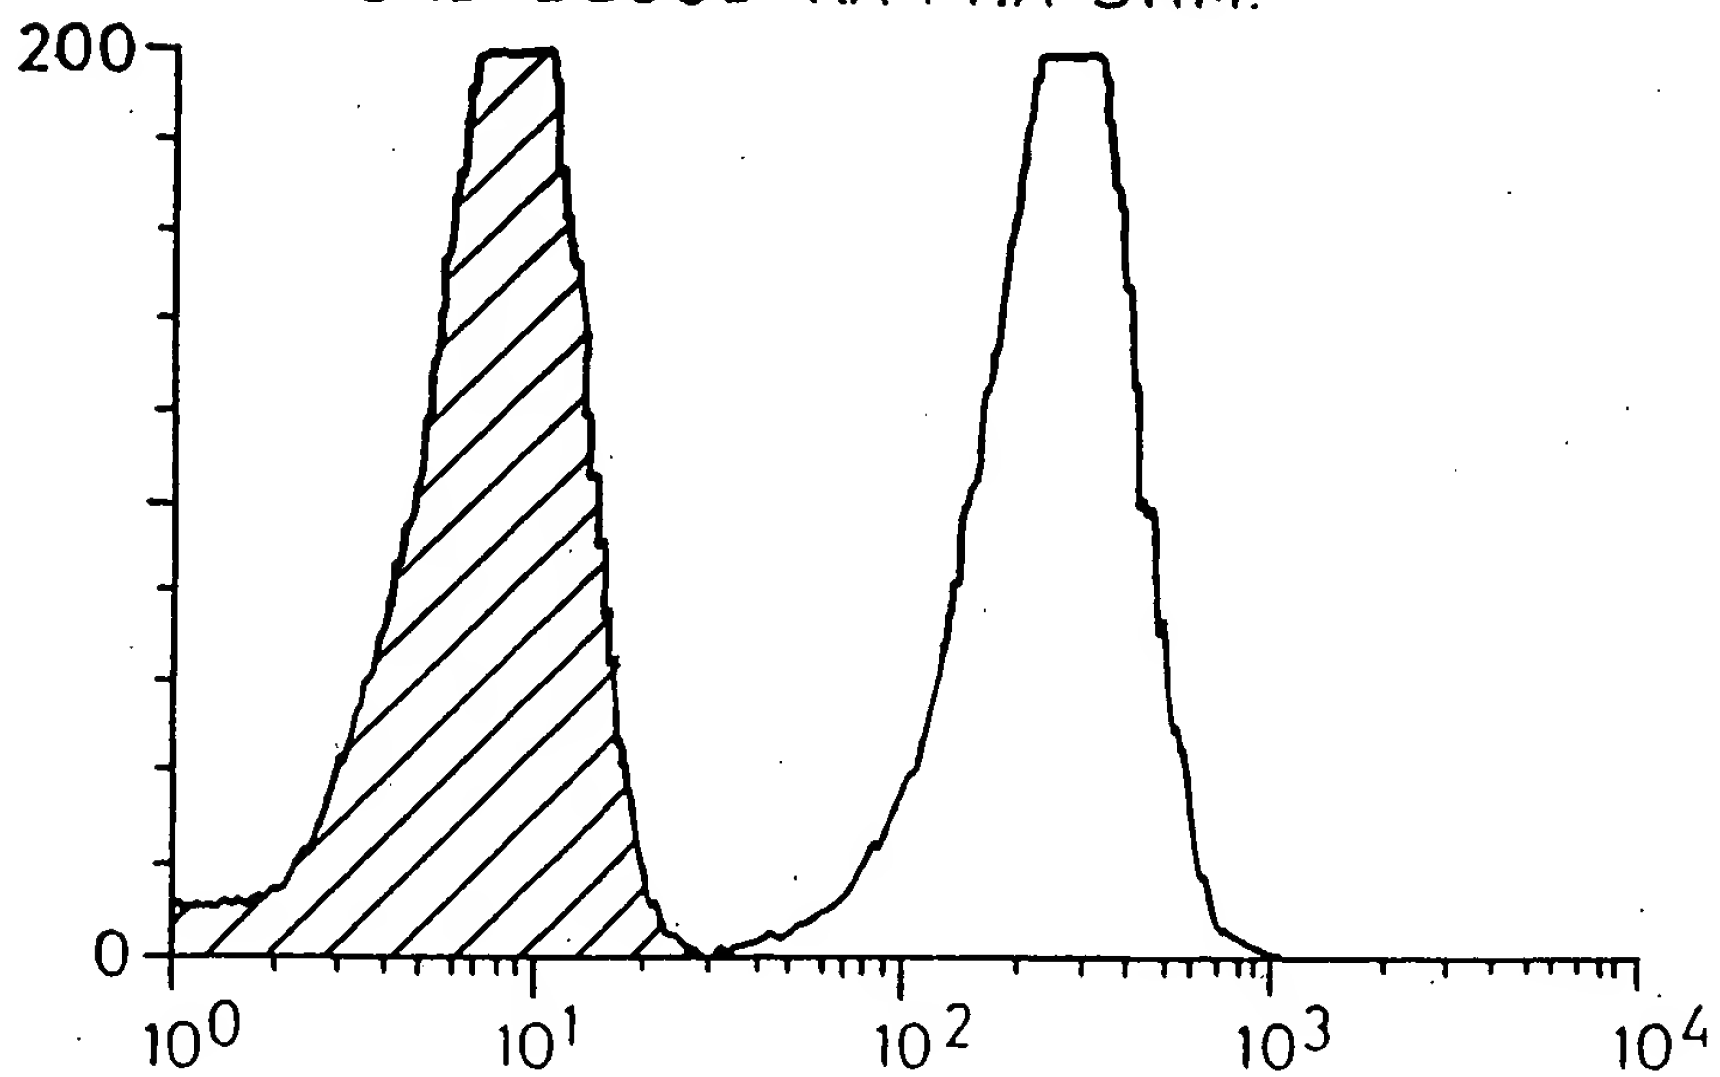


FIG. 3(D)

CORD BLOOD RA PHA STIM.



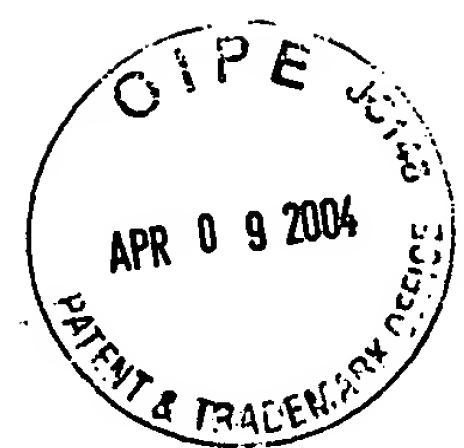


FIG. 3(E)

KC3 TCC



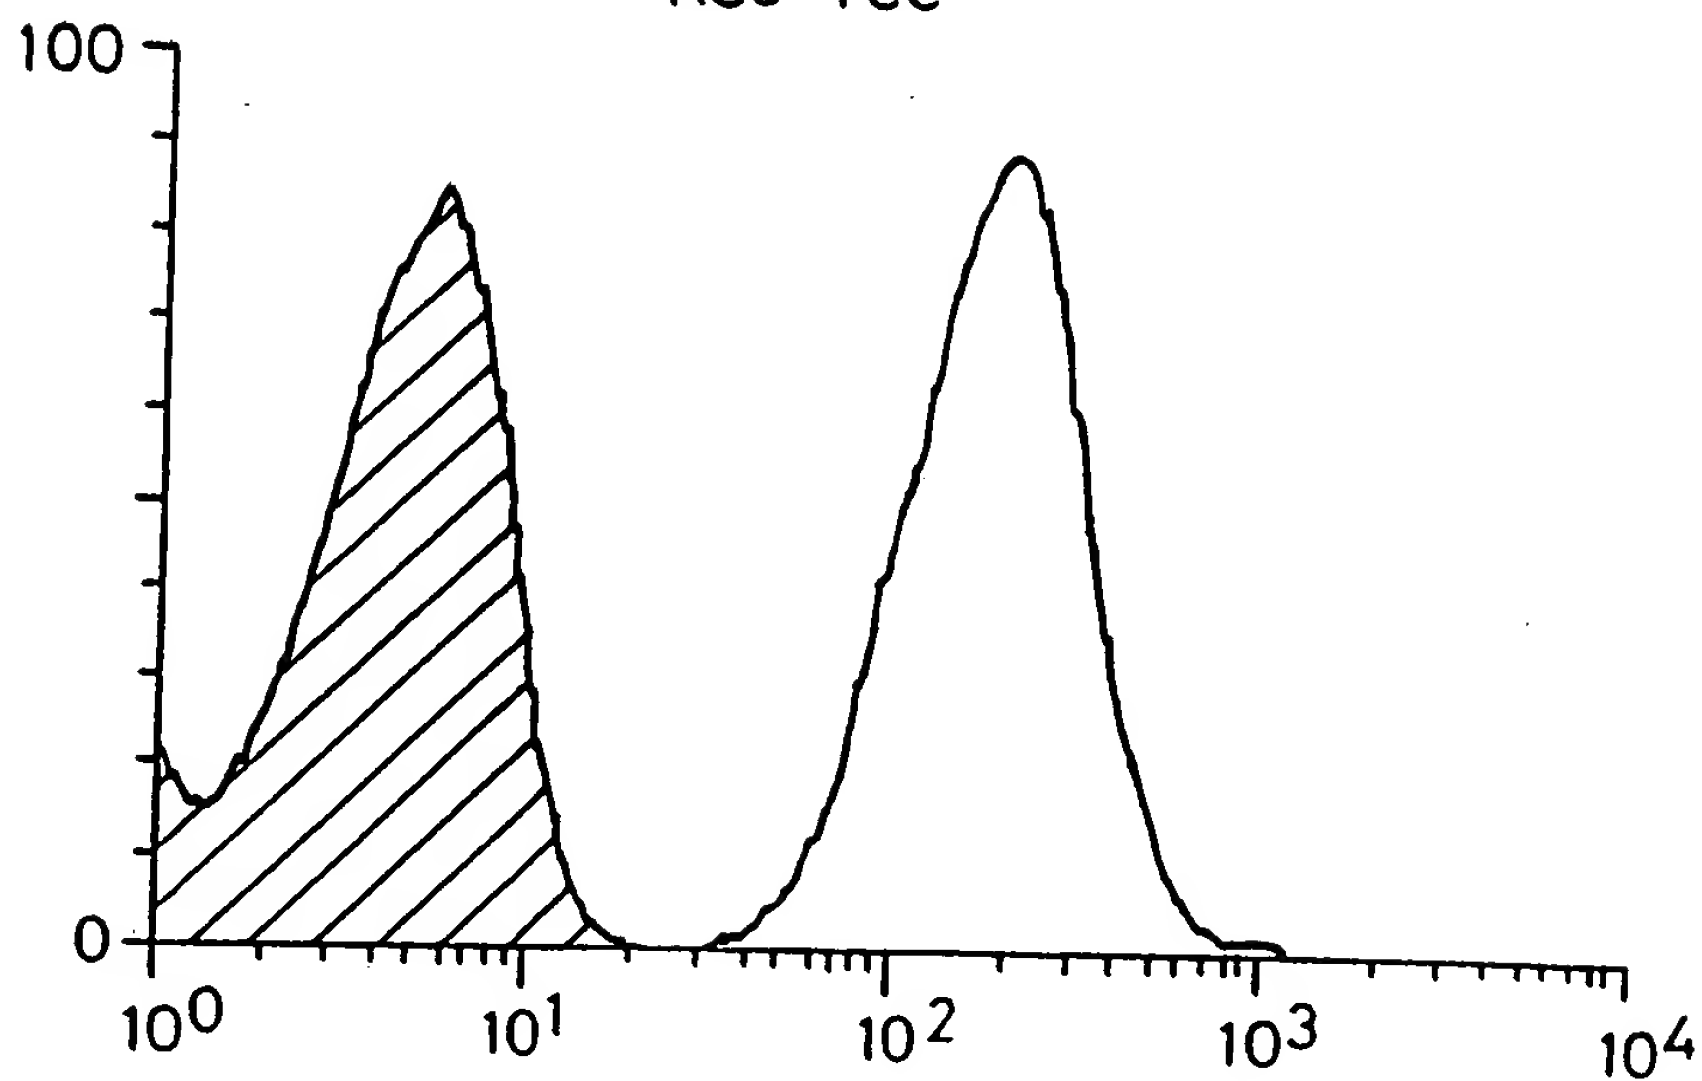


FIG. 3(F)

SAG S9 TCC

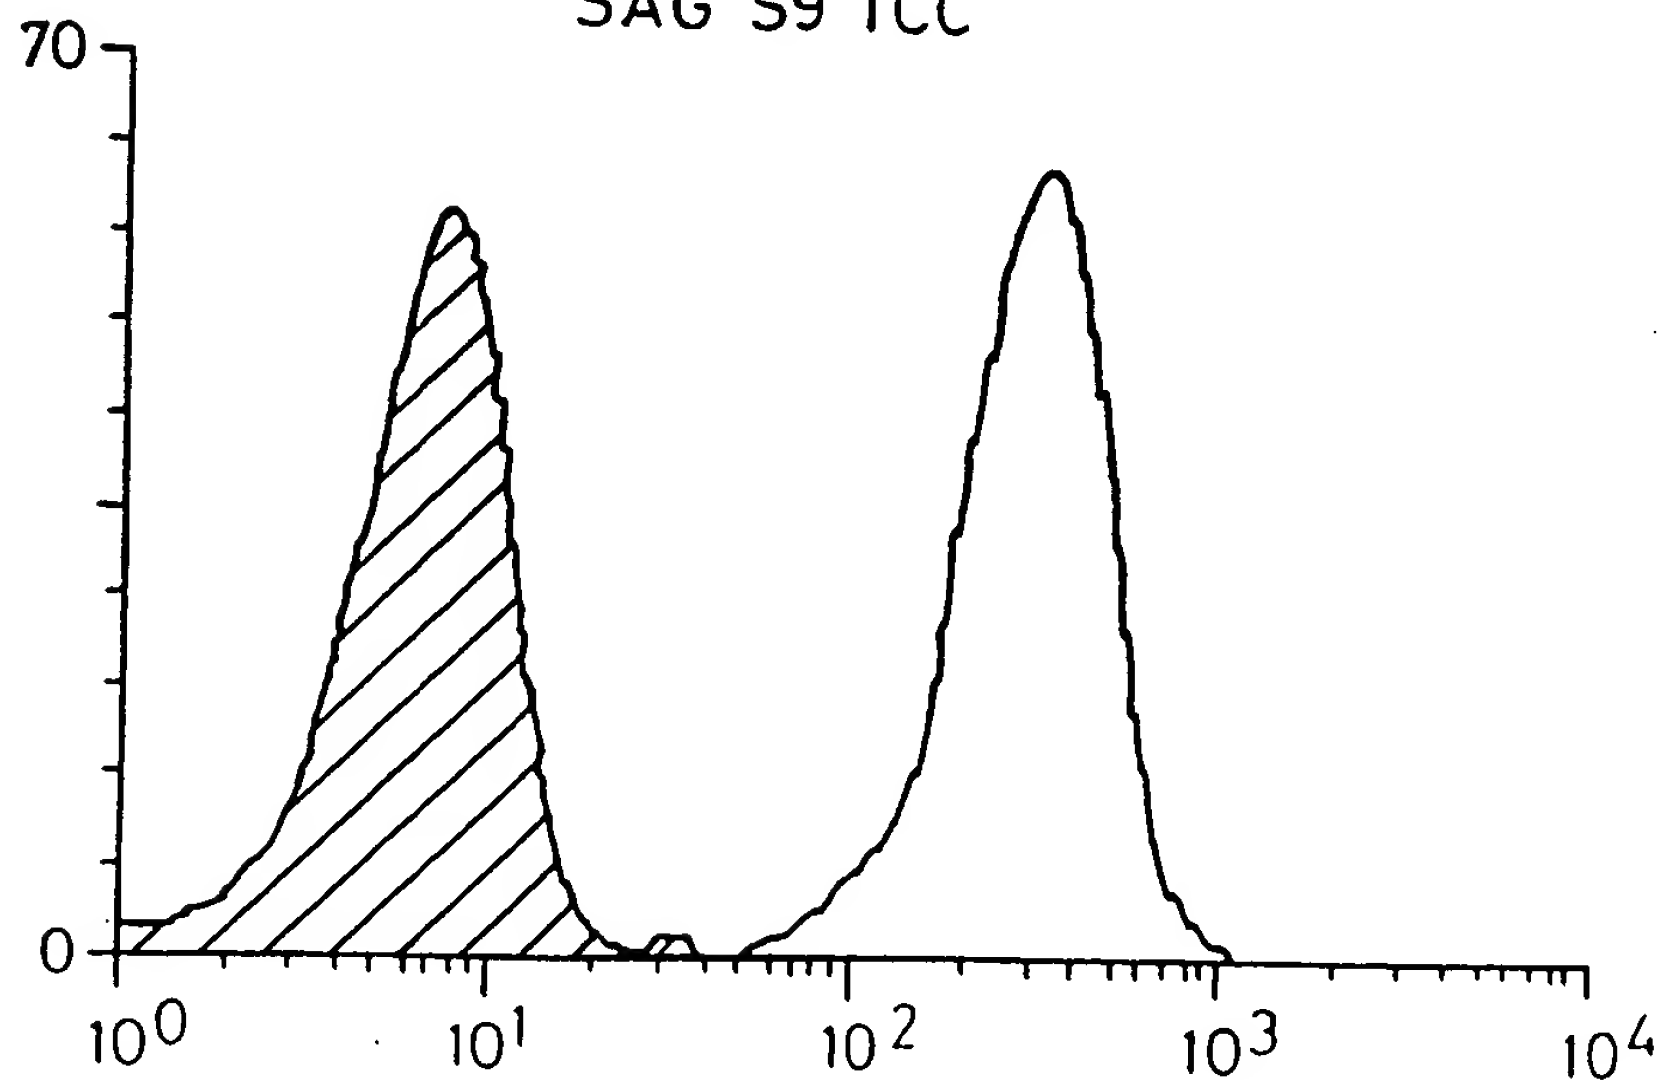

E2 CHO (CONF.)

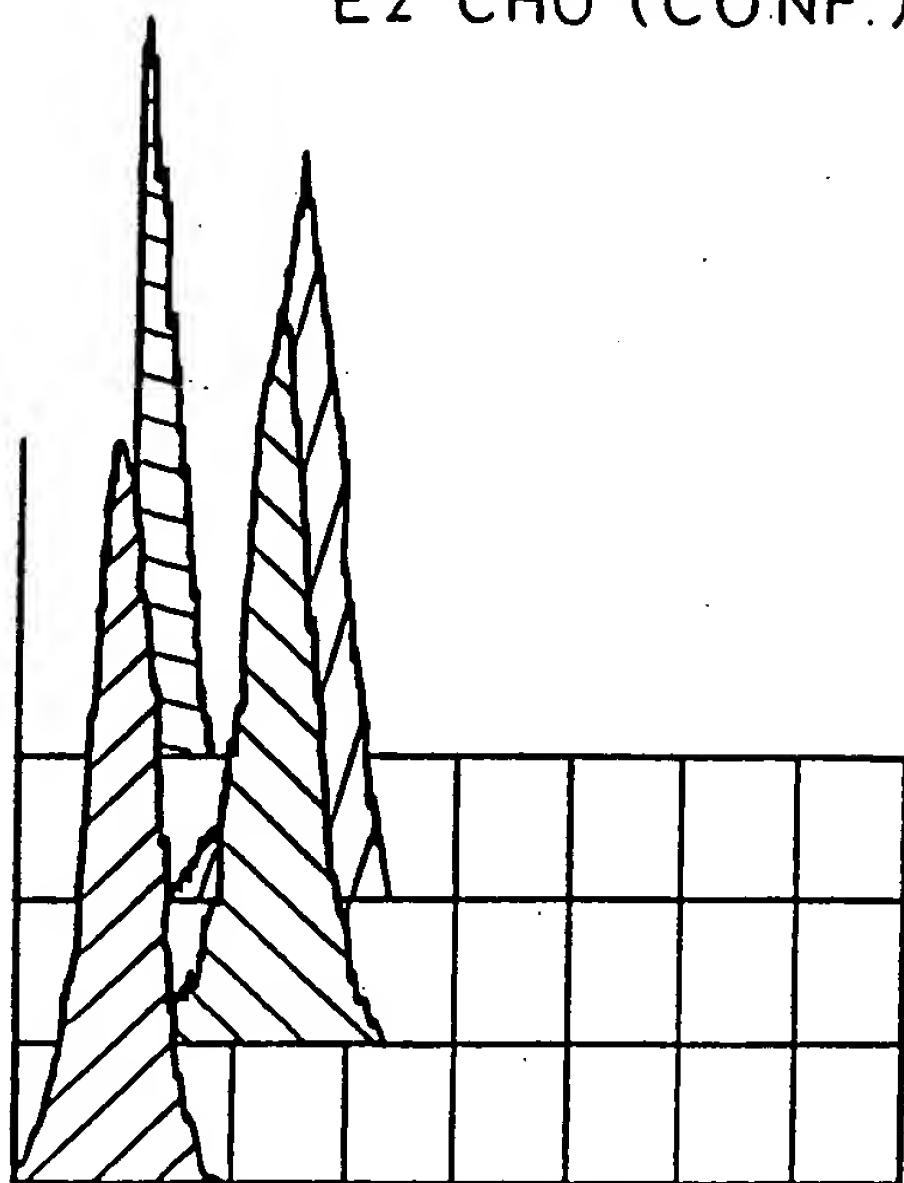

500 MM B-MERC.


BOILED (3 MIN.)

POSITIVE/CONTROL

NEGATIVE/CONTROL

FIG. 4

E2 CHO (CONF.)

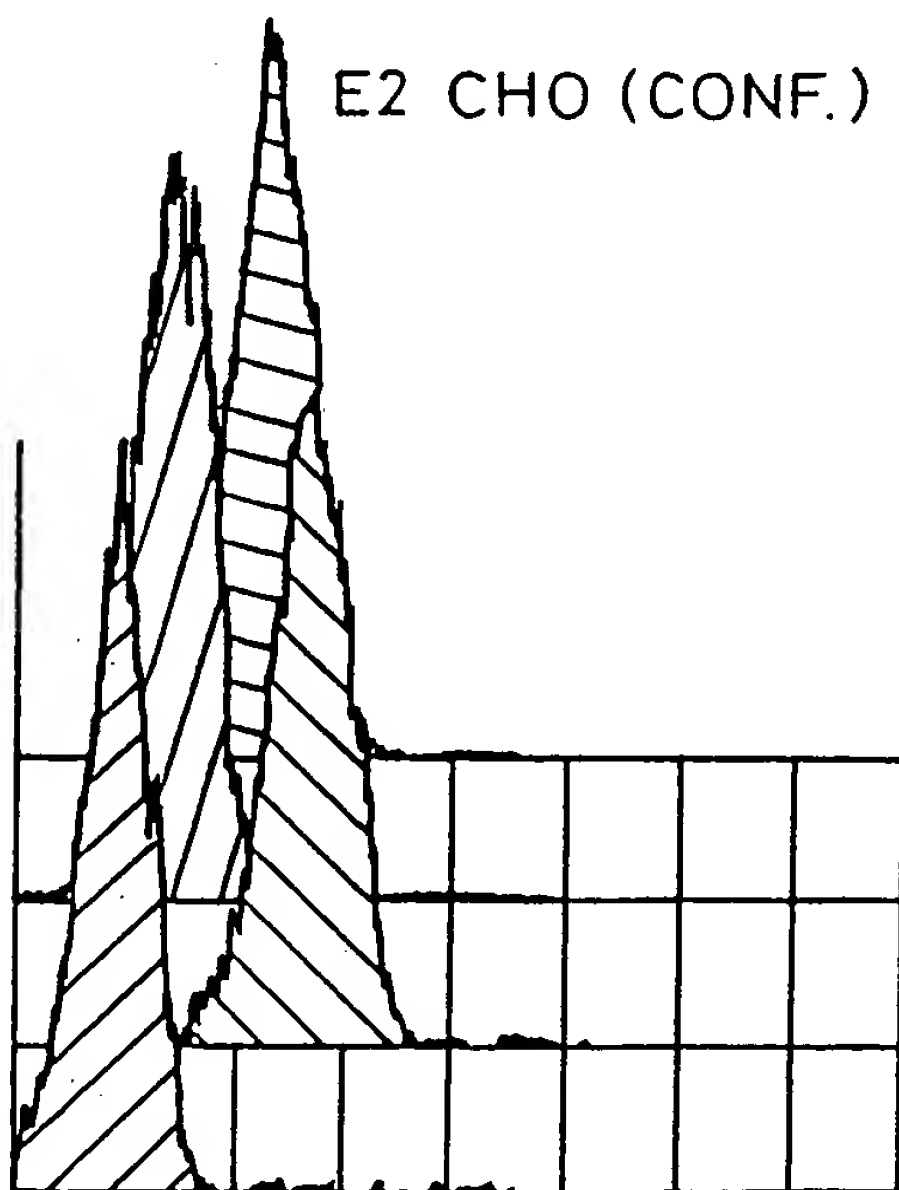

BOILED (10 MIN.)

0.2 U/ML ENDO H

POSITIVE/CONTROL

NEGATIVE CONTROL

FIG. 5

FIG. 6

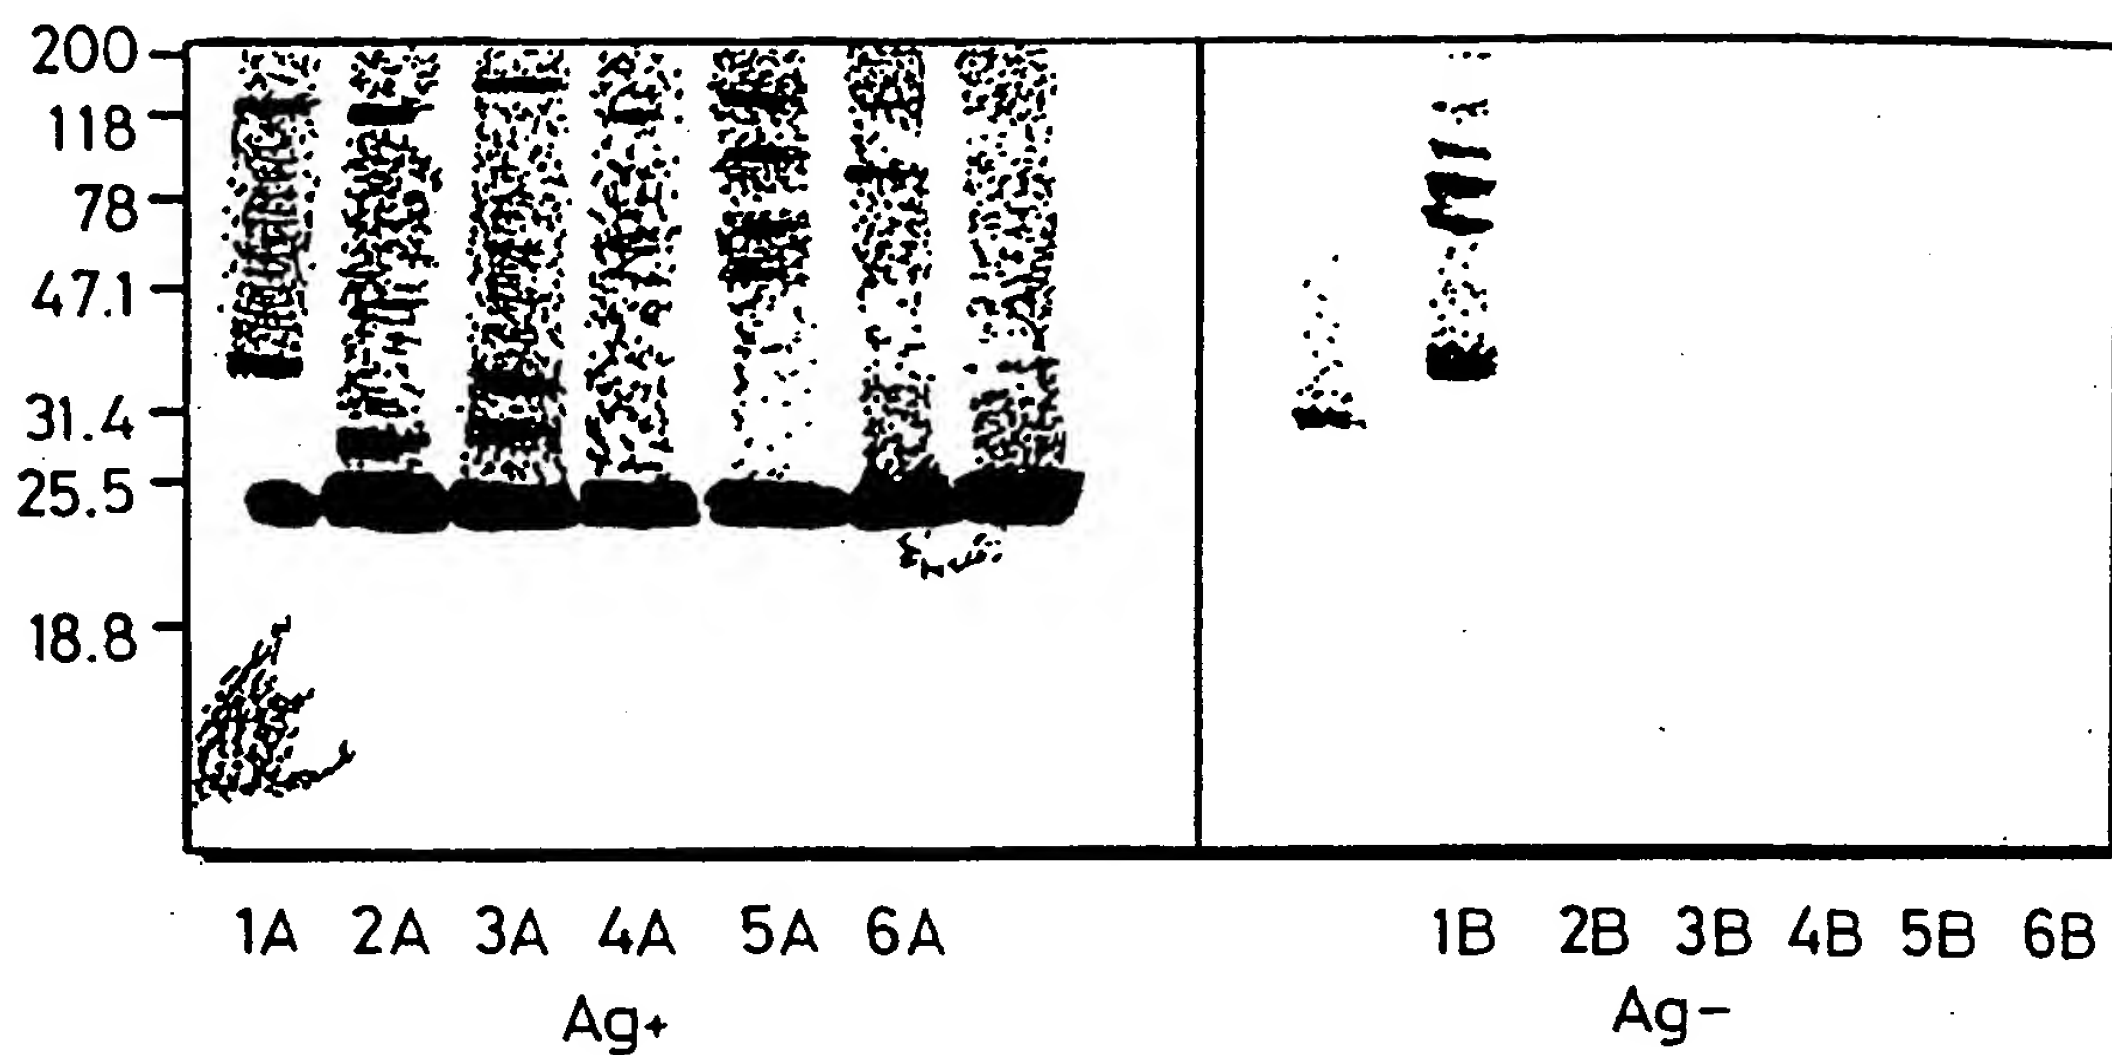


FIG. 7

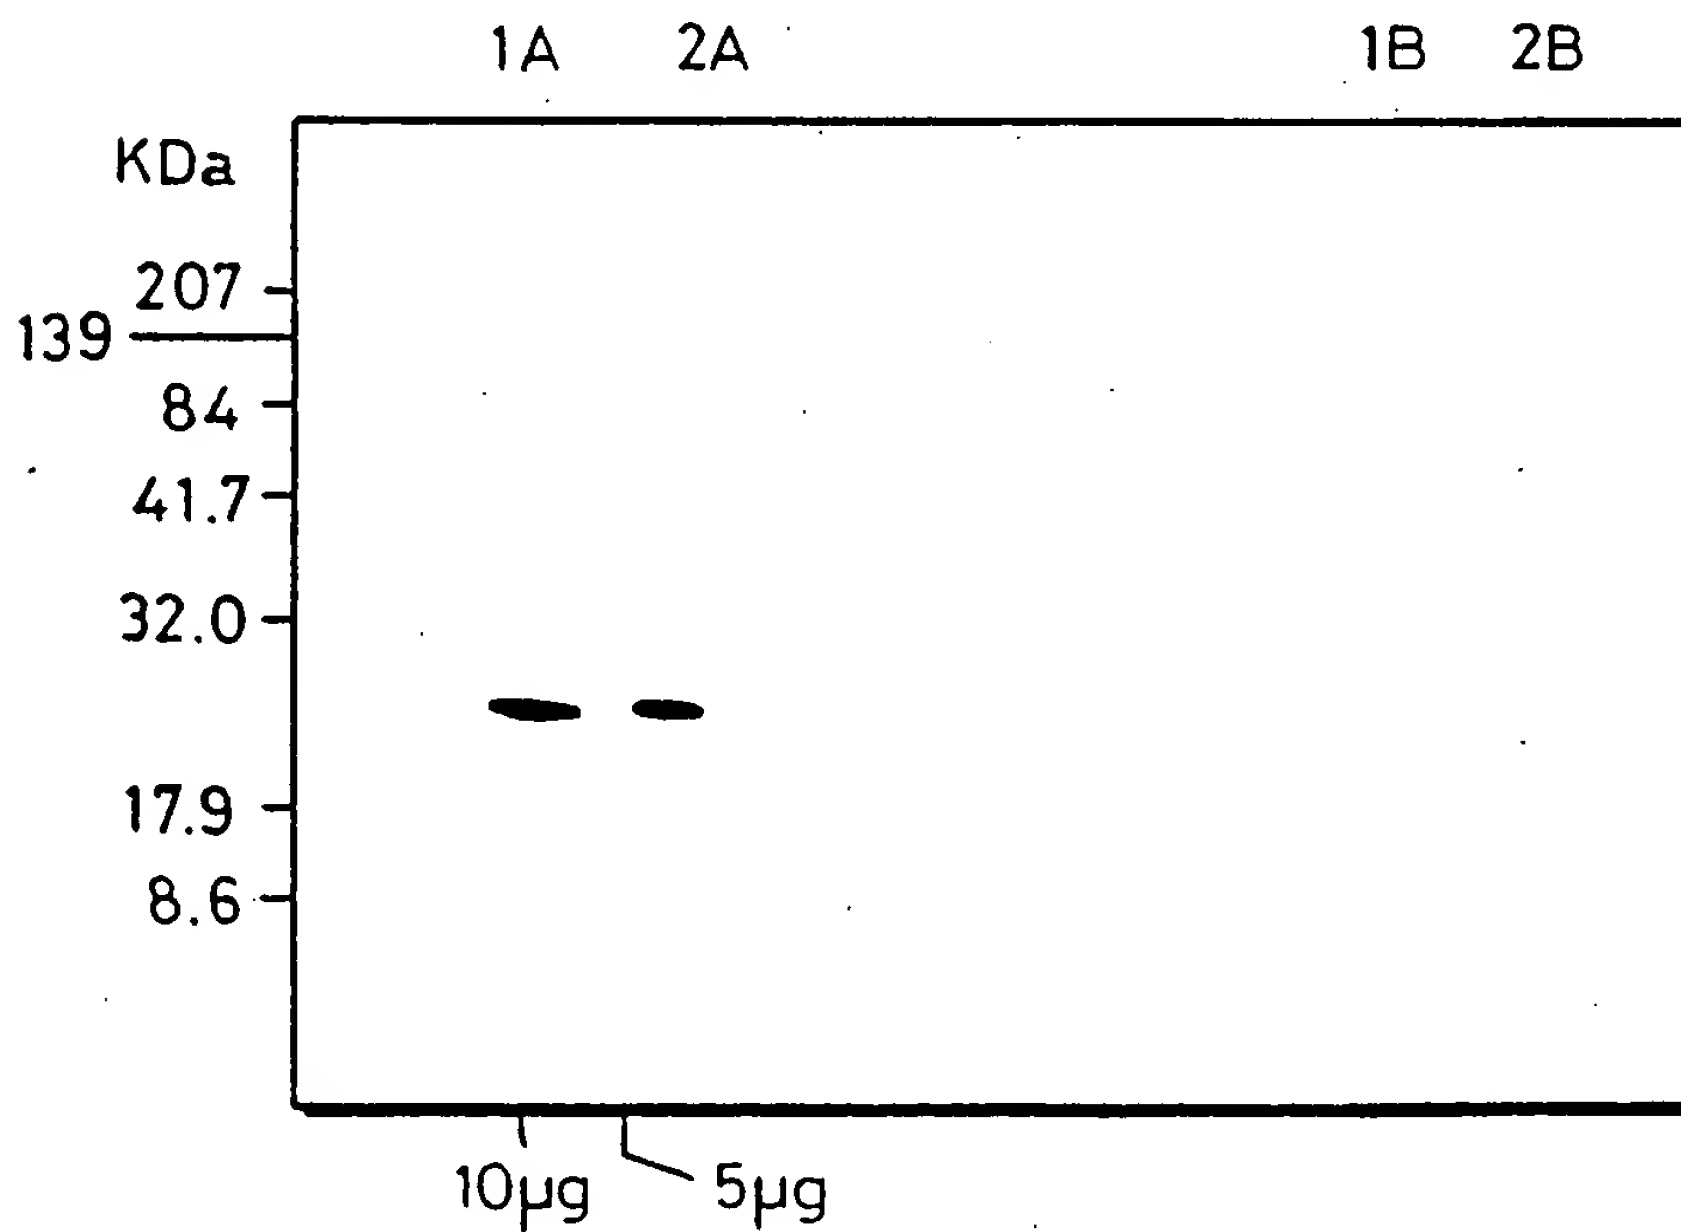


FIG. 8

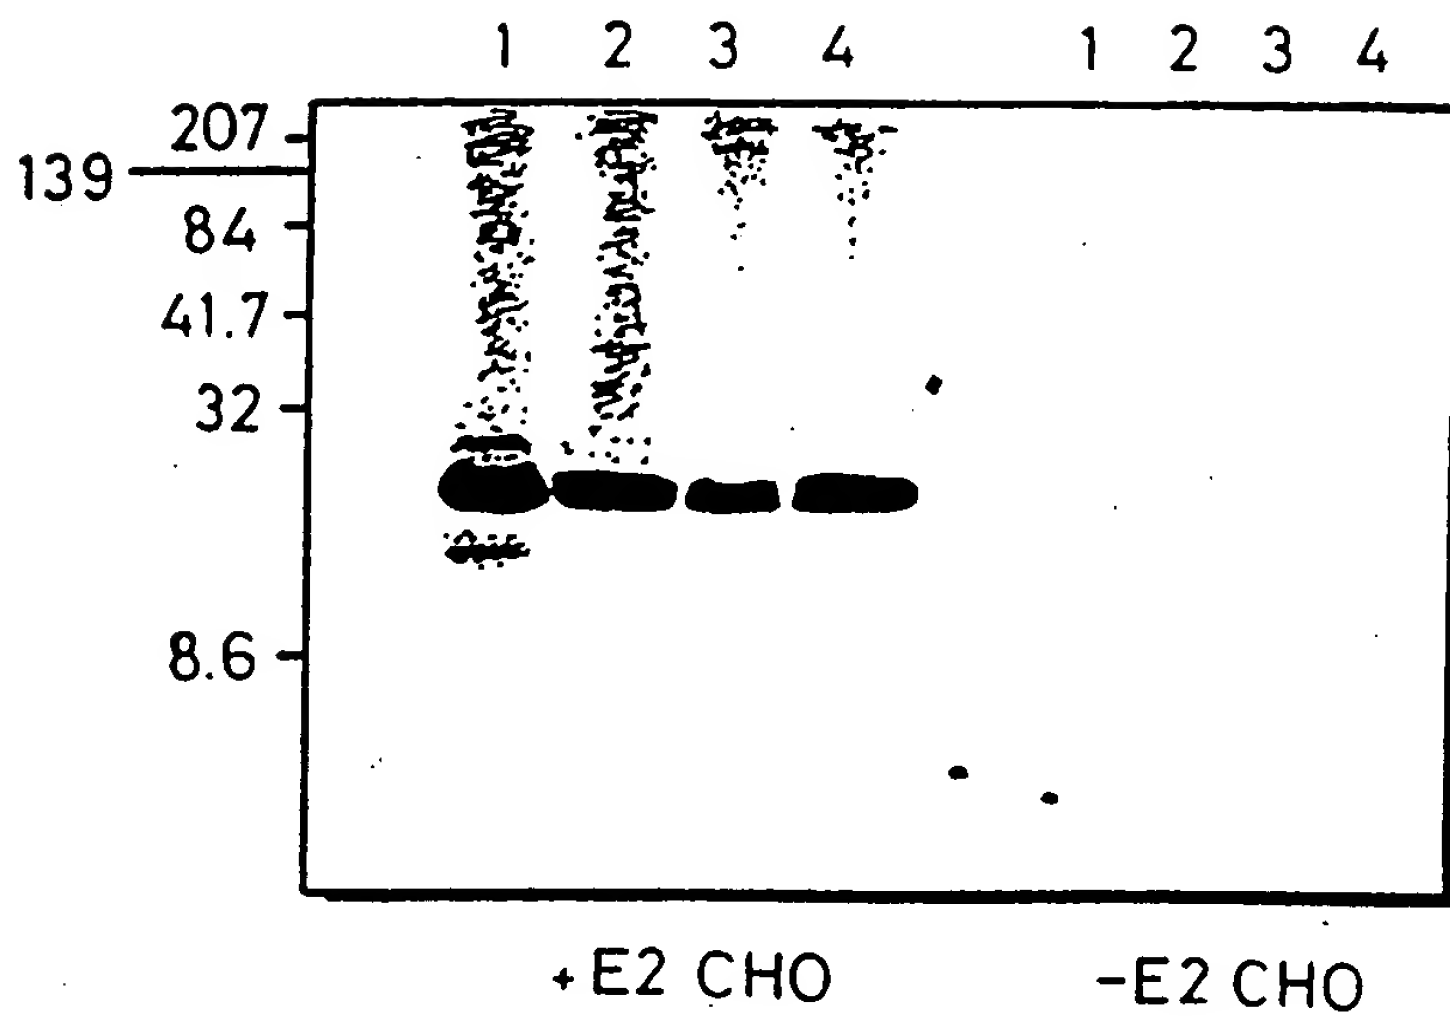


FIG. 9

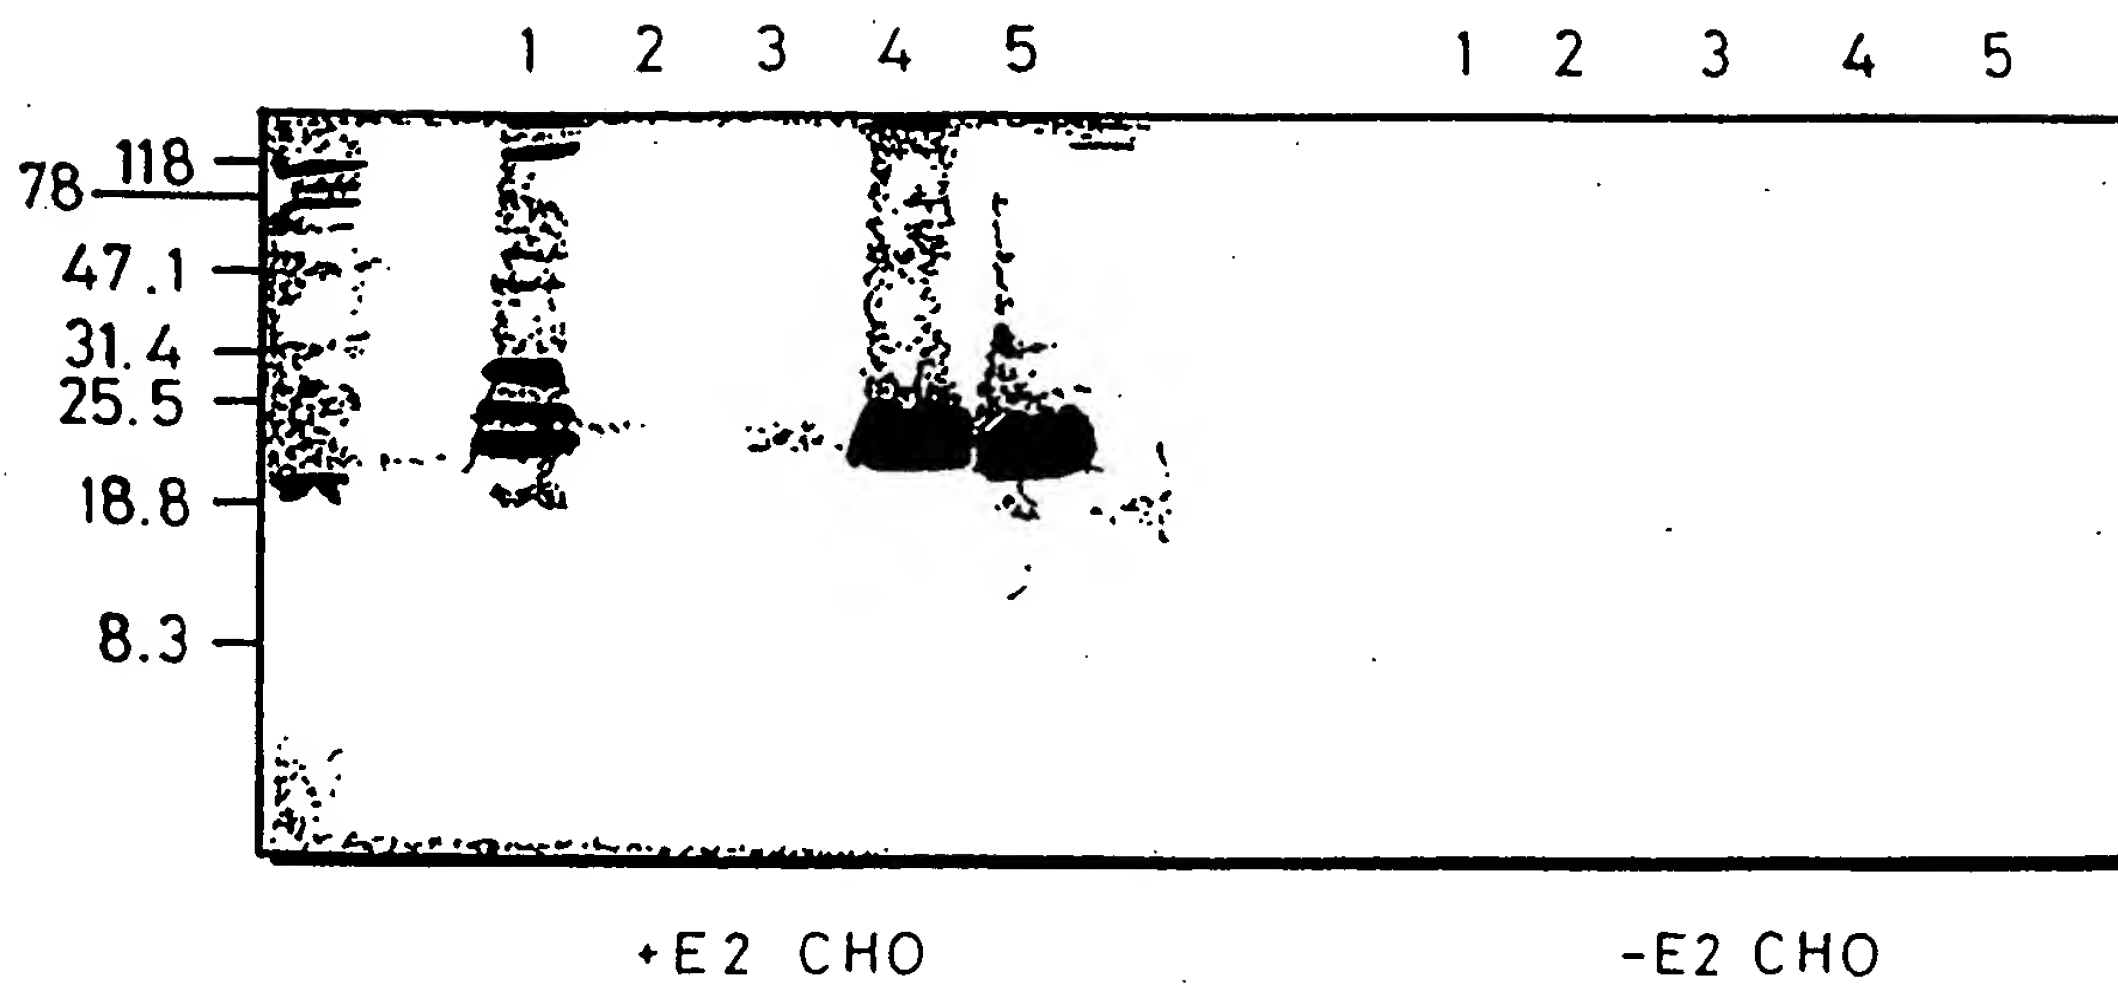


FIG. 10

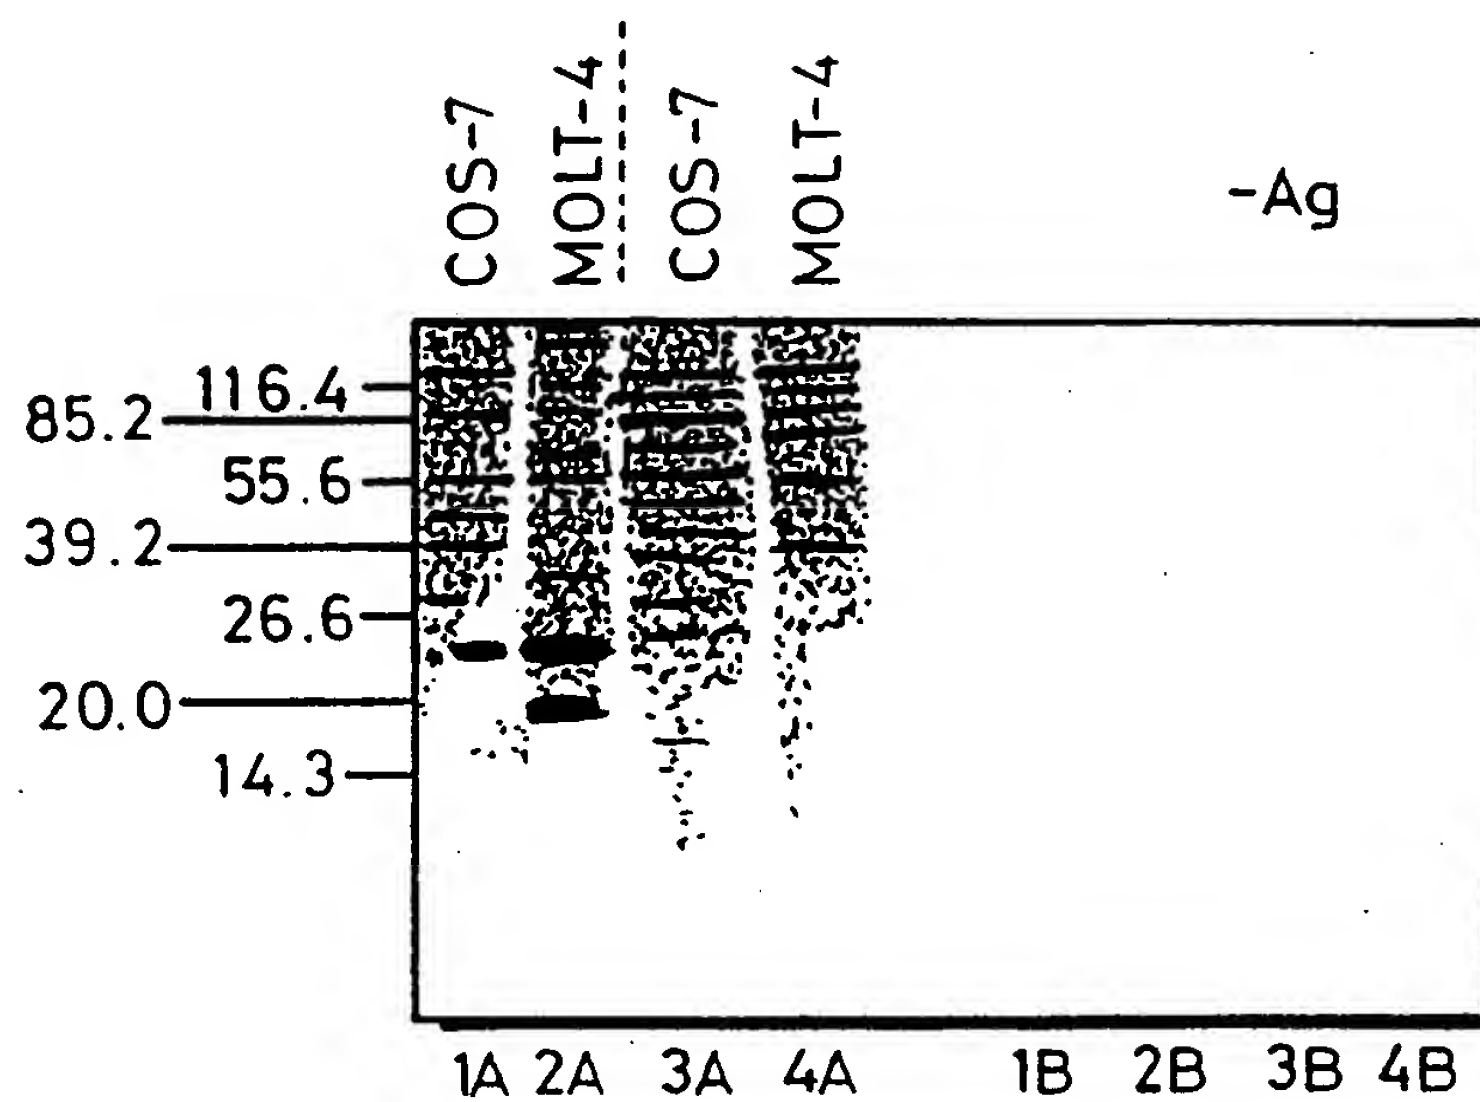


FIG. 11

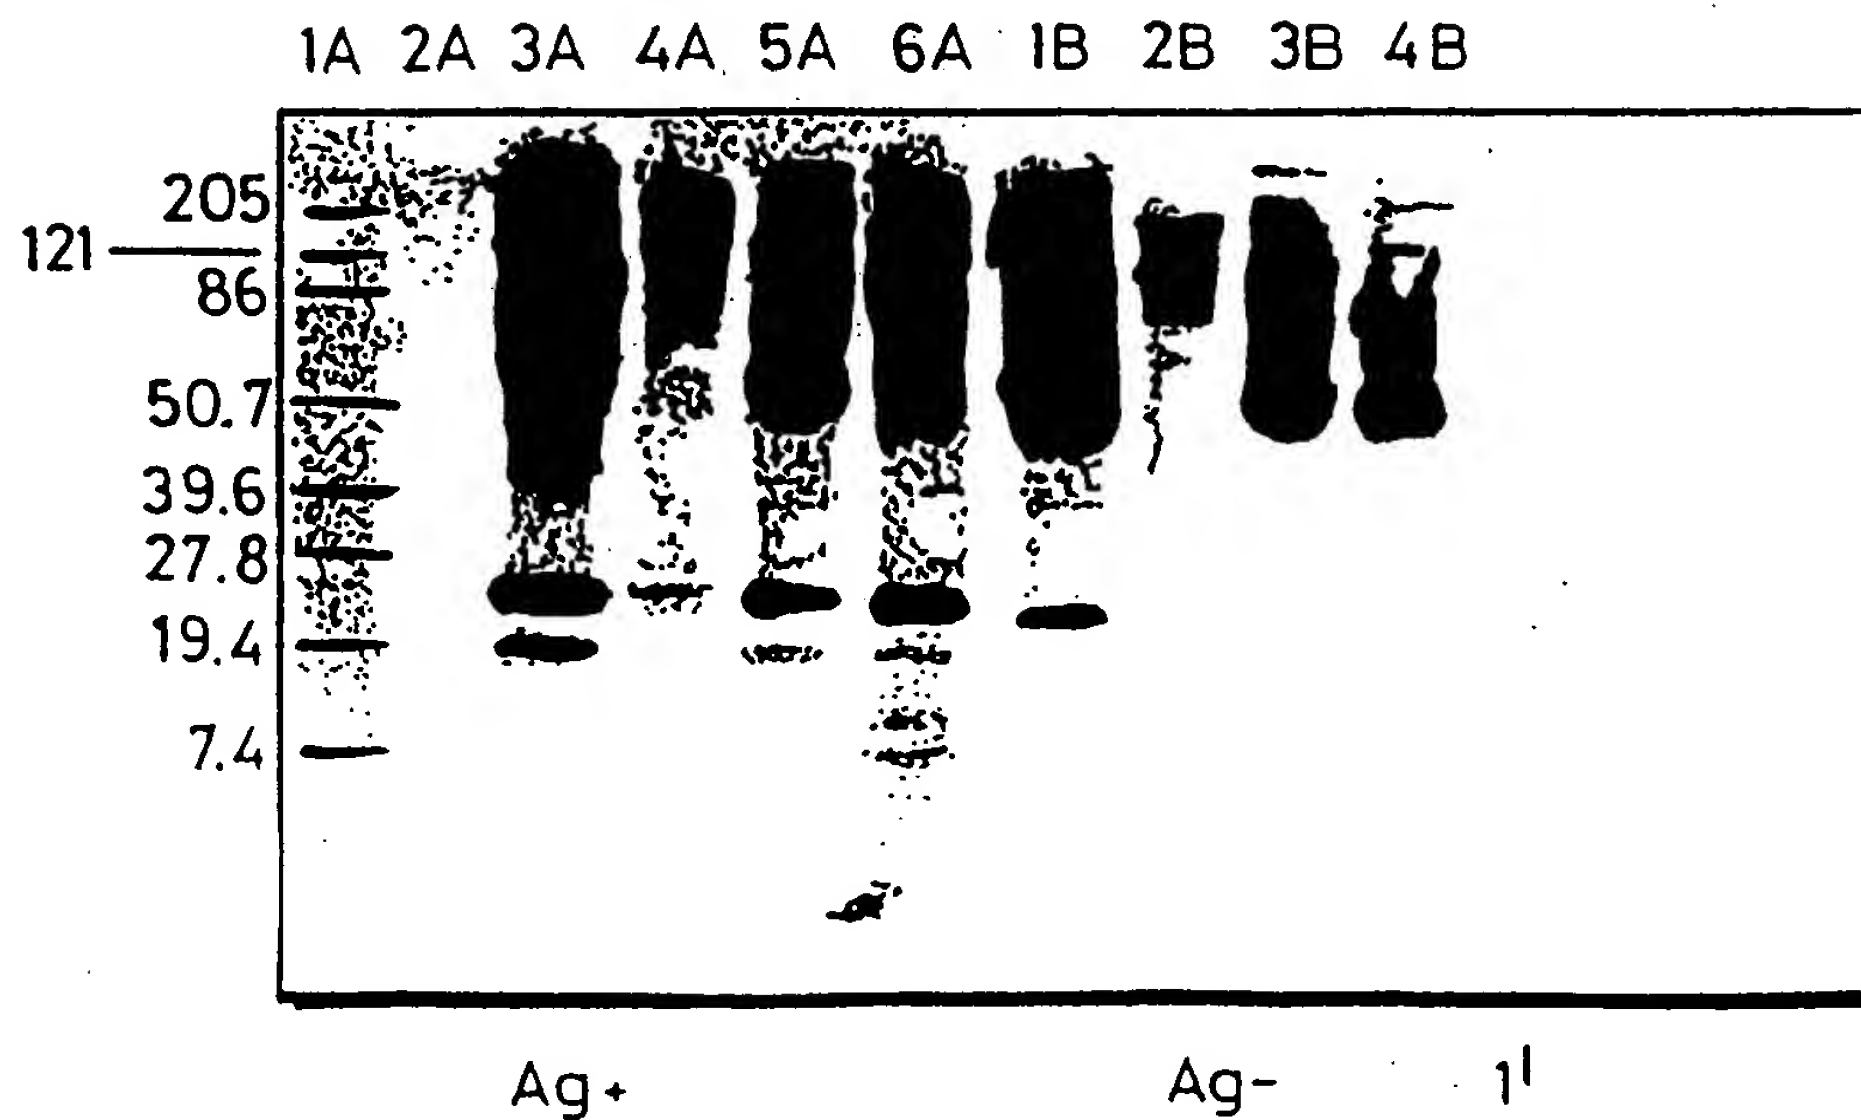


FIG. 12

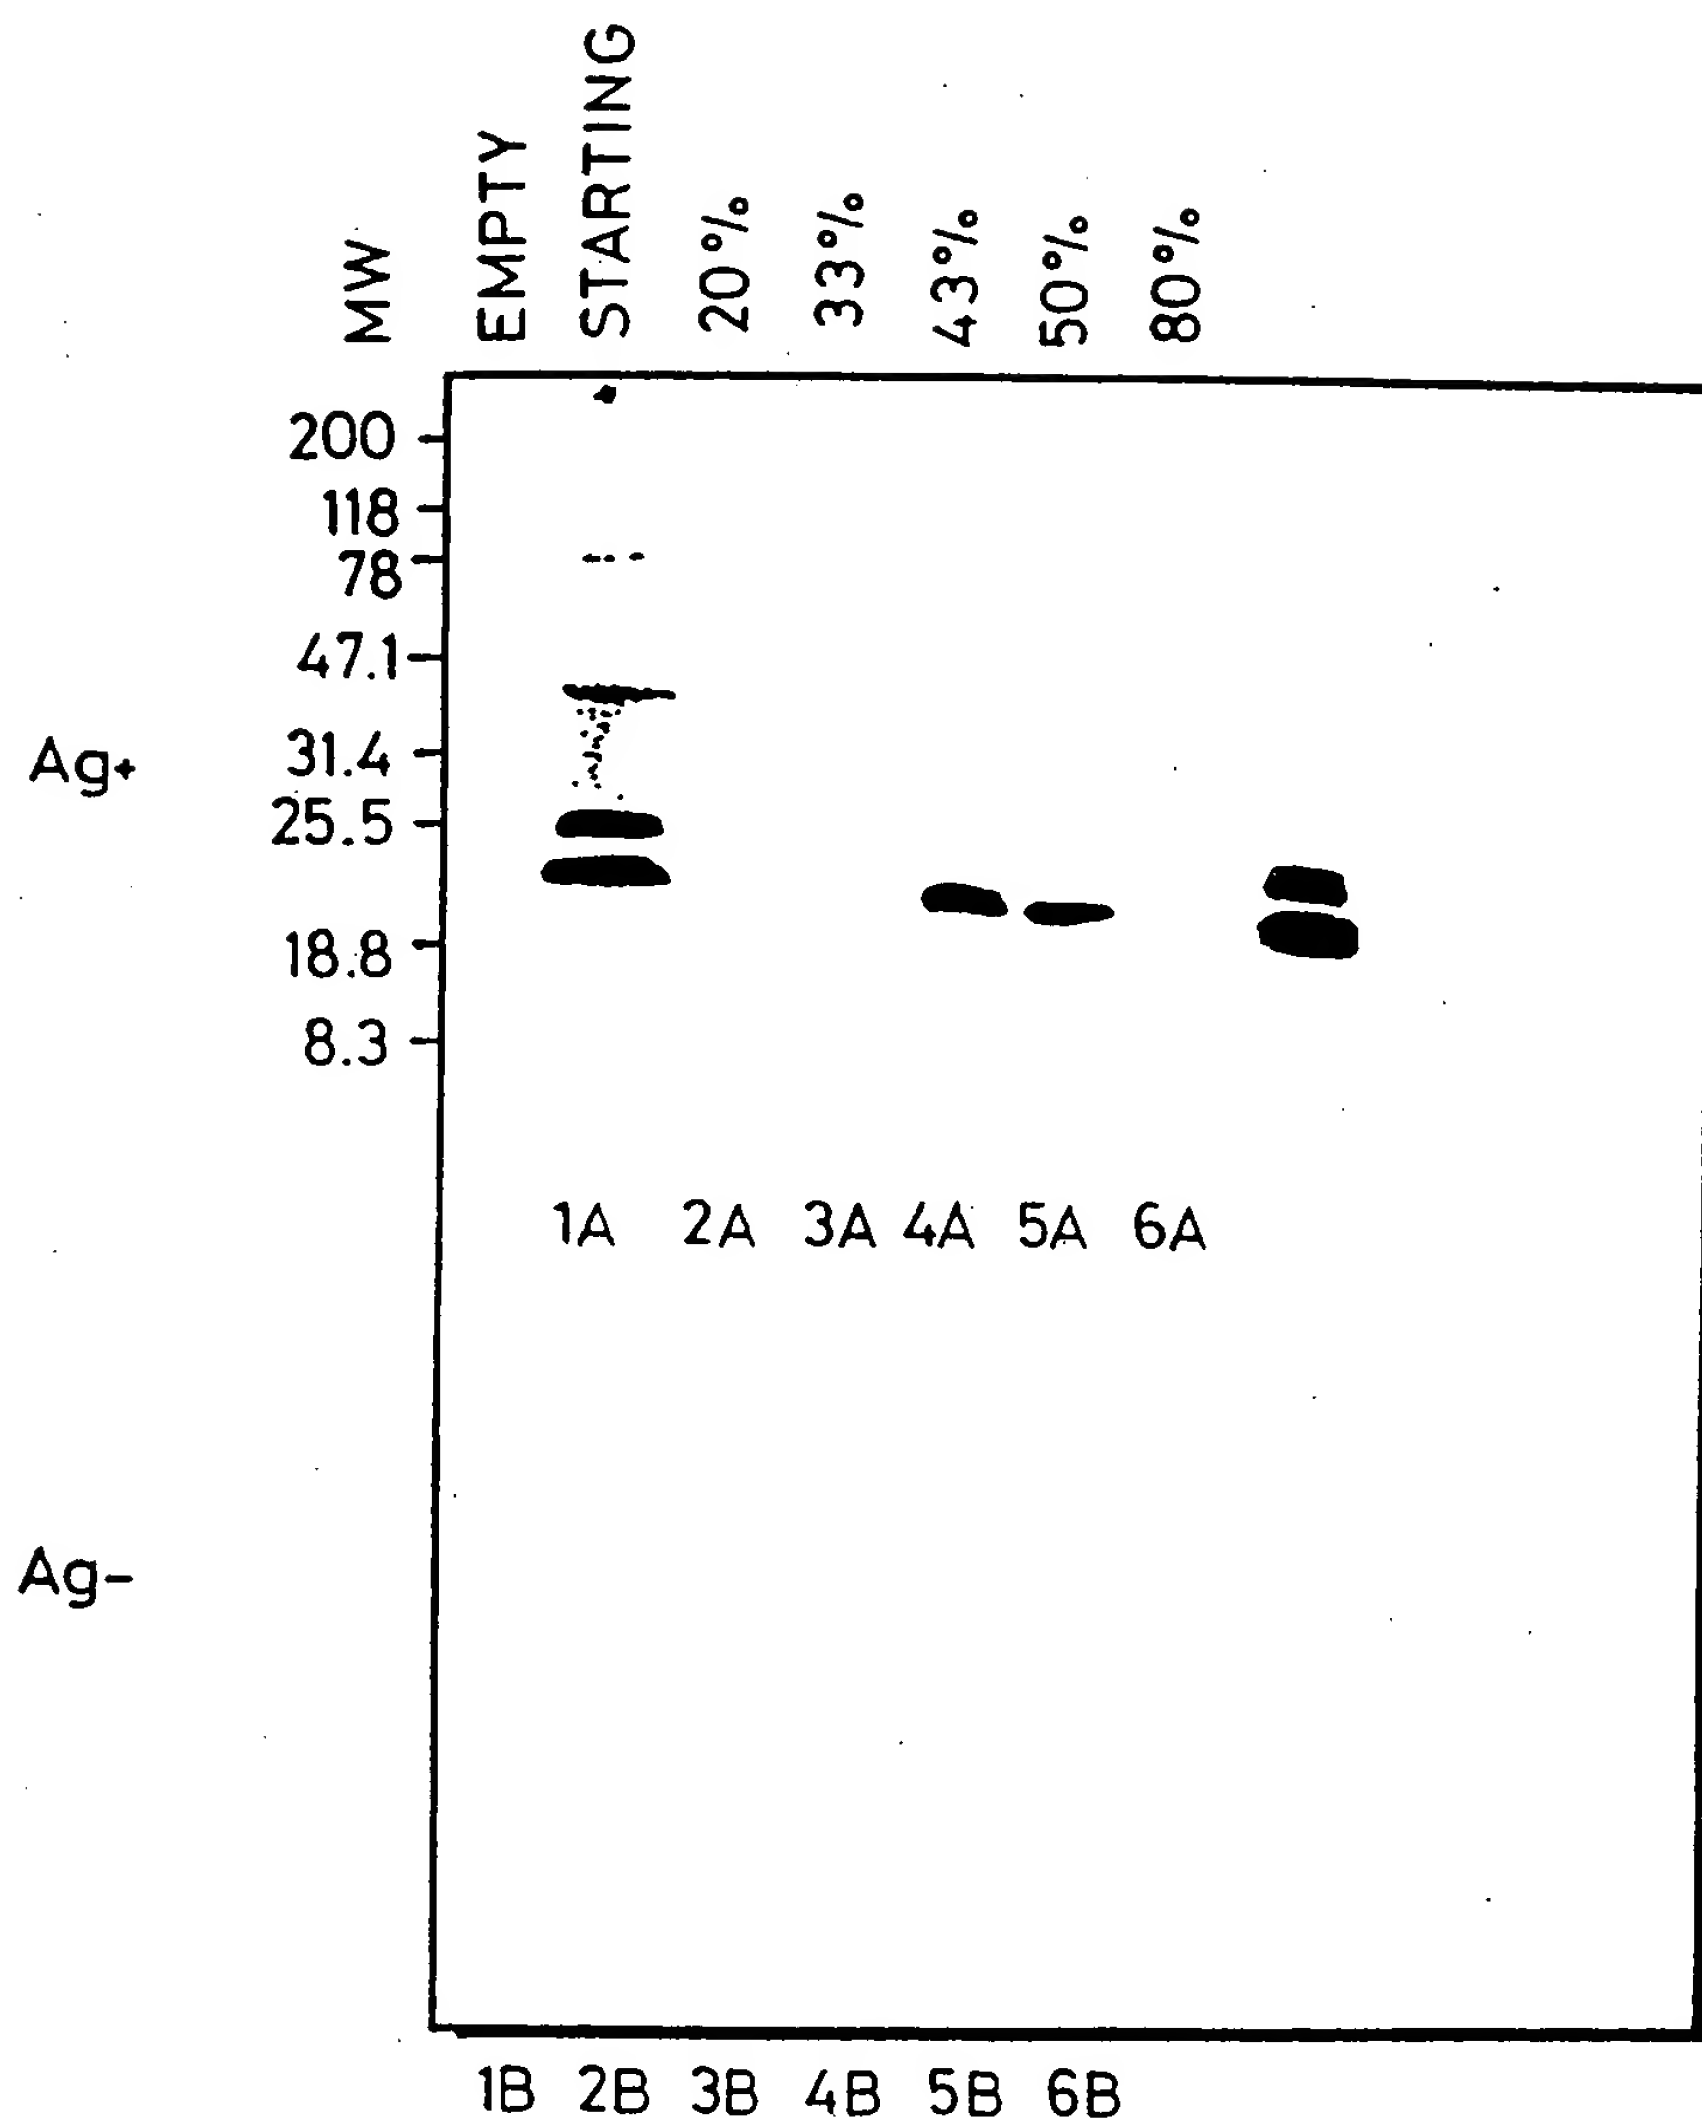




FIG. 13

